

Sample Name :HA Peptide
 Cat. No.: RP11735
 Lot. No. : E1095319G;
 Time Processed :12:15:06
 Month-Day-Year Processed : 07/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

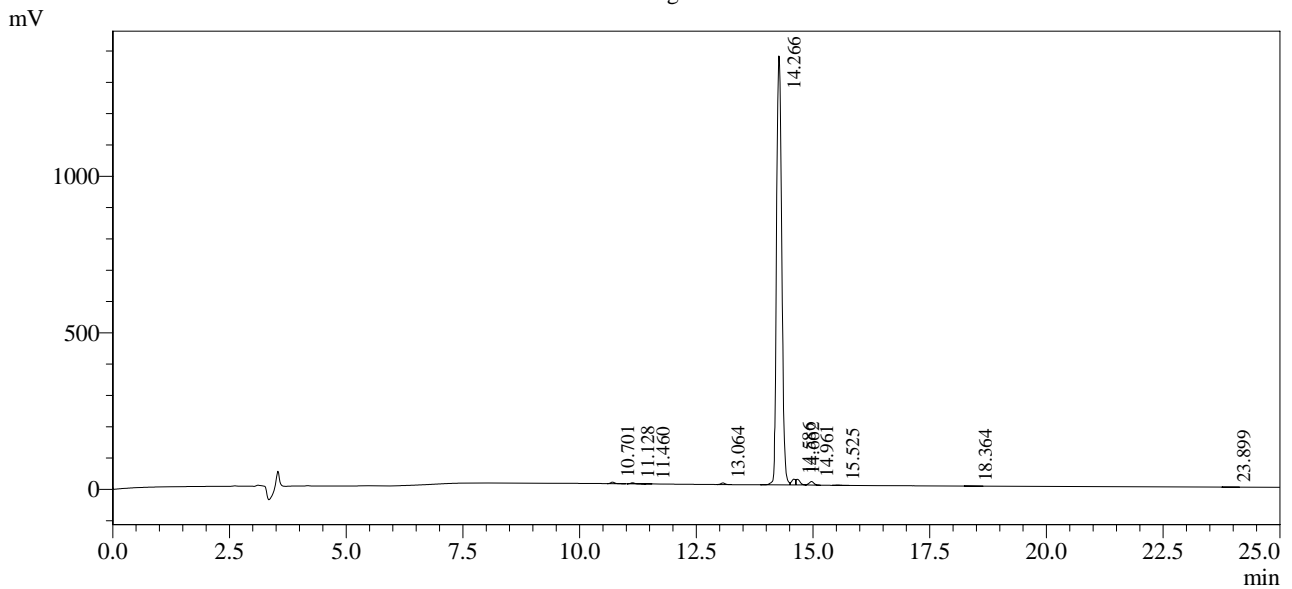

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.701	28158	4778	0.256
2	11.128	18418	3241	0.167
3	11.460	1106	280	0.010
4	13.064	33156	5293	0.301
5	14.266	10626703	1369930	96.594
6	14.586	108704	18208	0.988
7	14.662	97013	17677	0.882
8	14.961	76261	11078	0.693
9	15.525	7456	1028	0.068
10	18.364	2564	302	0.023
11	23.899	1867	178	0.017
Total		11001405	1431994	100.000