

Sample Name :OVA Peptide (257-264)
 Cat No :RP10611
 Lot No :E8443421B
 Time Processed :19:13:19
 Month-Day-Year Processed :02/10/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

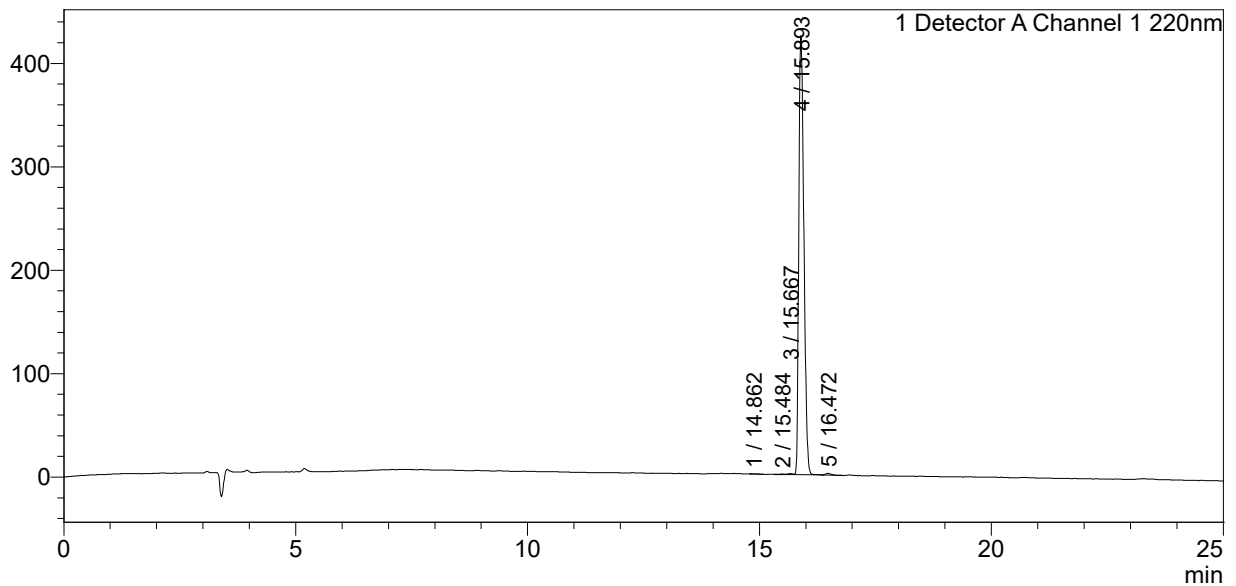

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.862	1987	153	0.061
2	15.484	4967	596	0.153
3	15.667	9024	1139	0.278
4	15.893	3218962	424642	99.075
5	16.472	14069	1601	0.433
Total		3249009	428131	100.000