

Sample Name :DYKDDDDK Peptide  
 Cat No.: RP10586  
 Lot No.:E9373920H  
 Time Processed :15:02:49  
 Month-Day-Year Processed :08/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	20
25.10	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
50.00	Pumps	Pump A B.Conc	15
51.00	Pumps	Pump A B.Conc	15
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

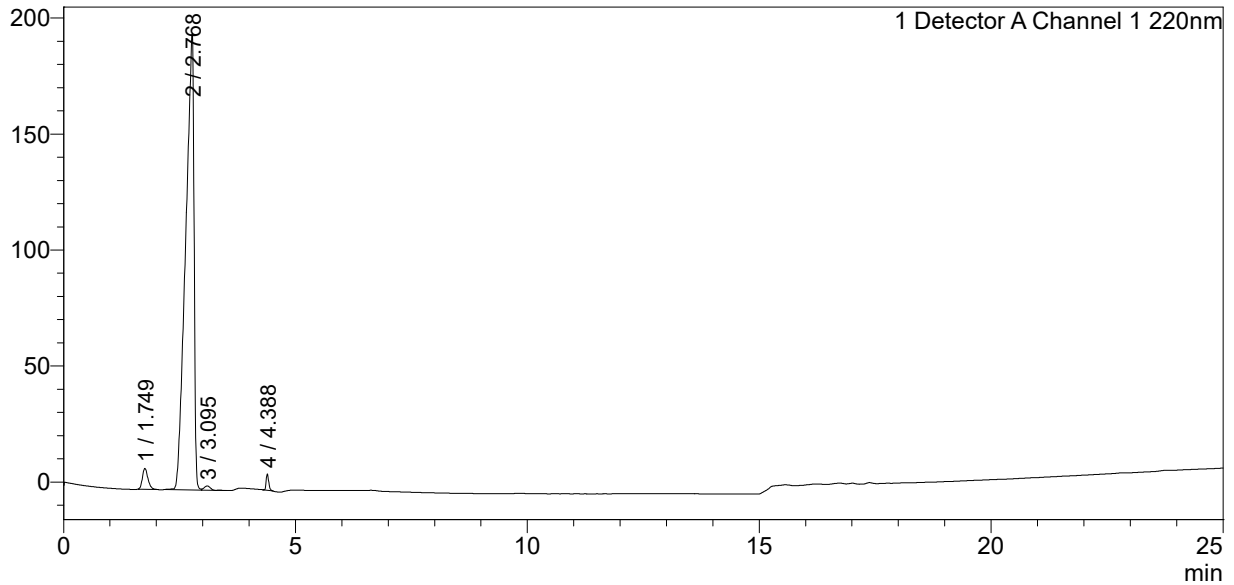

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	1.749	74568	9046	2.903
2	2.768	2450120	197025	95.388
3	3.095	17053	1856	0.664
4	4.388	26841	7049	1.045
Total		2568581	214975	100.000