

Sample Name :C-Peptide (3-33), human  
 Cat No :RP11116  
 Lot No :E8161020L  
 Time Processed :12:43:31 PM  
 Month-Day-Year Processed :12/27/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

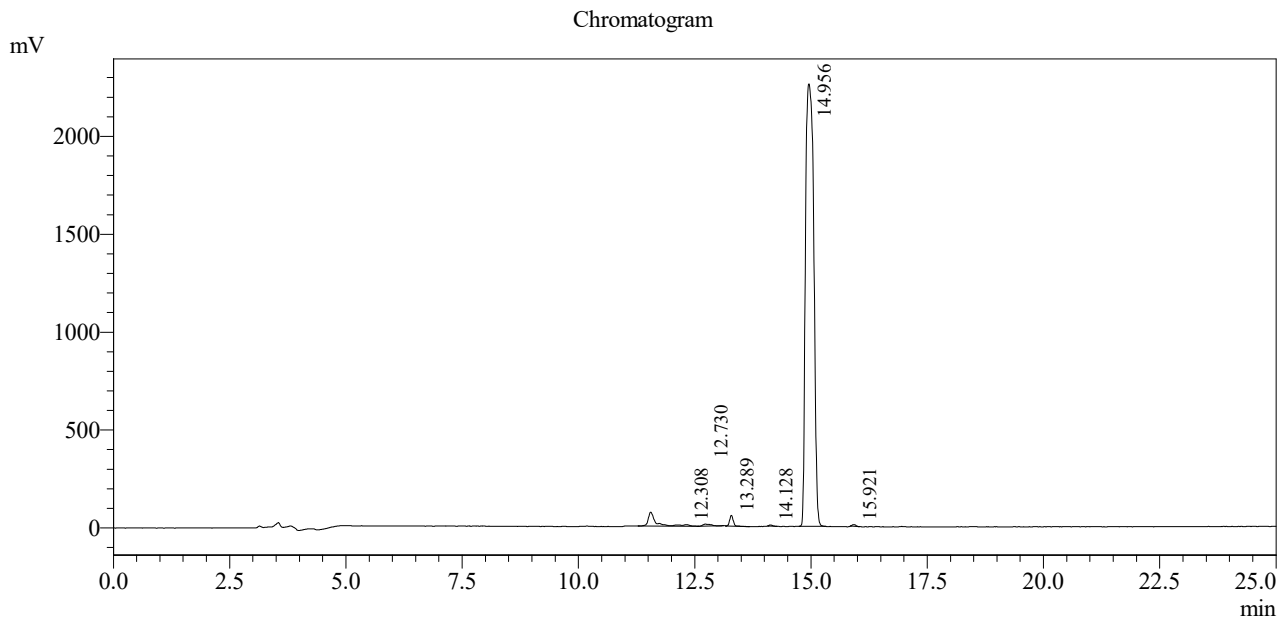

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.308	854665	7440	2.933
2	12.730	113125	10294	0.388
3	13.289	285733	54018	0.981
4	14.128	24387	5600	0.084
5	14.956	27811639	2259719	95.448
6	15.921	48335	8253	0.166
Total		29137885	2345323	100.000