

Sample Information

Sample Name :c-Myc Peptide  
 Cat. No :RP11731  
 Lot. No. :PE4661806

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>  
 Flow : 1.0000 mL/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>  
 <Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm

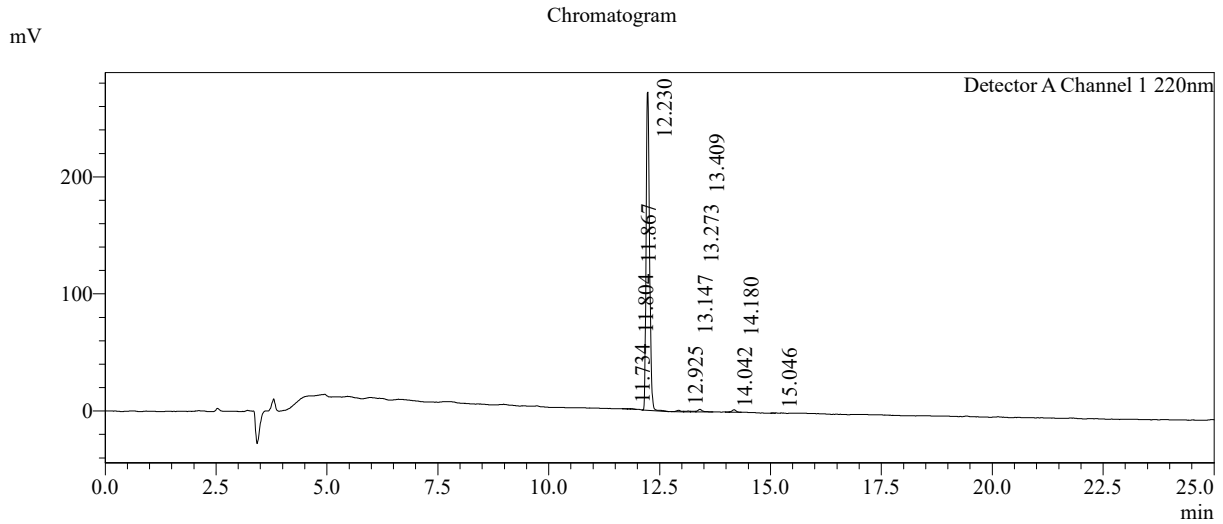

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	11.734	263	1425	0.094	0.093
2	11.804	355	1336	0.127	0.087
3	11.867	419	1495	0.150	0.098
4	12.230	271648	1474557	96.996	96.413
5	12.925	1153	8285	0.412	0.542
6	13.147	608	4618	0.217	0.302
7	13.273	635	4064	0.227	0.266
8	13.409	2149	16314	0.767	1.067
9	14.042	389	1553	0.139	0.102
10	14.180	2198	14741	0.785	0.964
11	15.046	245	1030	0.088	0.067
Total		280062	1529416	100.000	100.000