

Sample Name : α -MSH, amide
 Cat No. :RP10644
 Lot No. :PE4301902
 Time Processed :9:00:40
 Month-Day-Year Processed :02/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

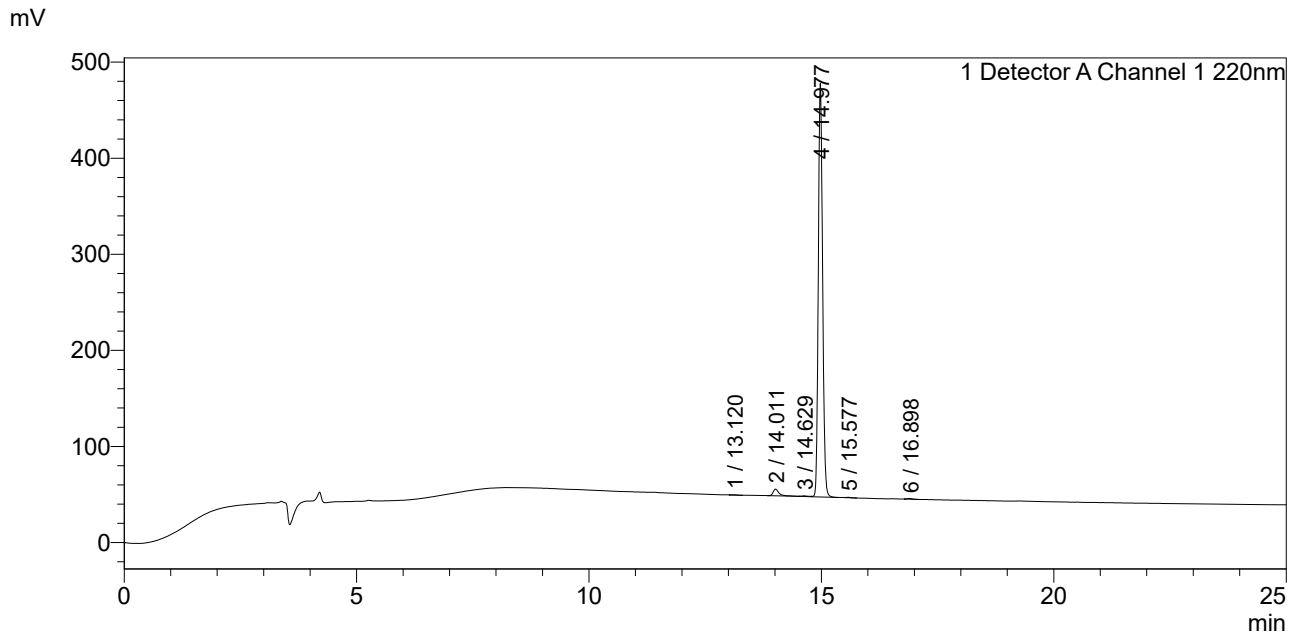

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.120	3175	505	0.112
2	14.011	61033	6987	2.149
3	14.629	6432	674	0.226
4	14.977	2760866	430282	97.221
5	15.577	3101	522	0.109
6	16.898	5186	739	0.183
Total		2839794	439709	100.000