

Sample Name :DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. :E2540519H
 Time Processed :7:39:15 PM
 Month-Day-Year
 Processed :08/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

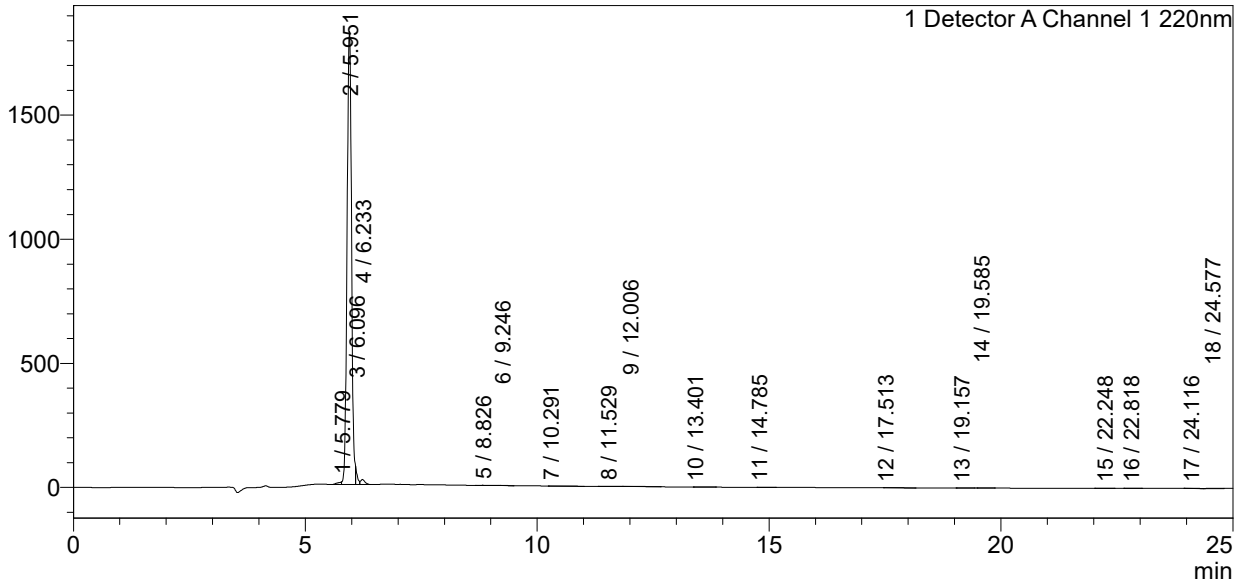

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.779	57180	9123	0.456
2	5.951	12145737	1824896	96.789
3	6.096	165124	64235	1.316
4	6.233	123722	19692	0.986
5	8.826	8459	446	0.067
6	9.246	1829	138	0.015
7	10.291	7532	98	0.060
8	11.529	3304	176	0.026
9	12.006	15707	433	0.125
10	13.401	2752	59	0.022
11	14.785	1595	53	0.013
12	17.513	3760	138	0.030
13	19.157	1509	106	0.012
14	19.585	1027	99	0.008
15	22.248	1905	152	0.015

Peak#	Ret. Time	Area	Height	Area%
16	22.818	1077	98	0.009
17	24.116	2686	213	0.021
18	24.577	3772	277	0.030
Total		12548677	1920432	100.000