

Sample Name :Gastric Inhibitory Peptide (GIP), human  
 Cat. No. : RP10795  
 Lot. No. : E7091921A

Time Processed :6:51:21  
 Month-Day-Year Processed :01/15/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: SS-CM-0309

<Chromatogram>

mV

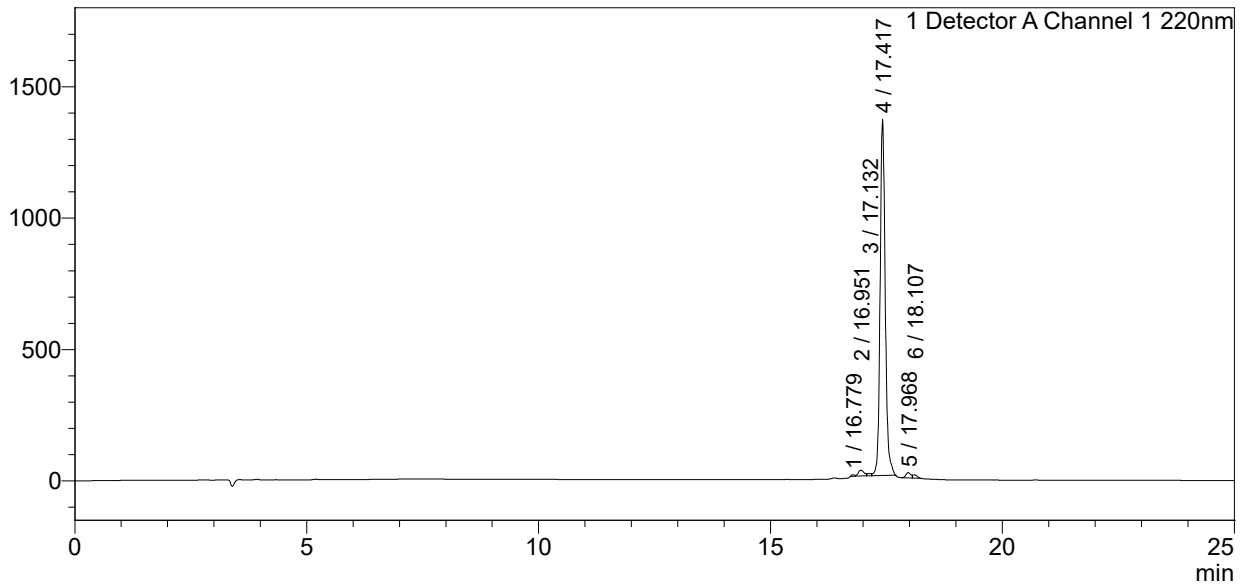

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.779	27434	5830	0.250
2	16.951	196895	22477	1.794
3	17.132	53930	8847	0.491
4	17.417	10463711	1353858	95.334
5	17.968	149206	20120	1.359
6	18.107	84709	12807	0.772
Total		10975885	1423939	100.000