

Sample Name :LL37 (Human)
 Cat. No. : RP13323
 Lot. No. : E2004921A
 Time Processed :2:39:06 AM
 Month-Day-Year Processed :01/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

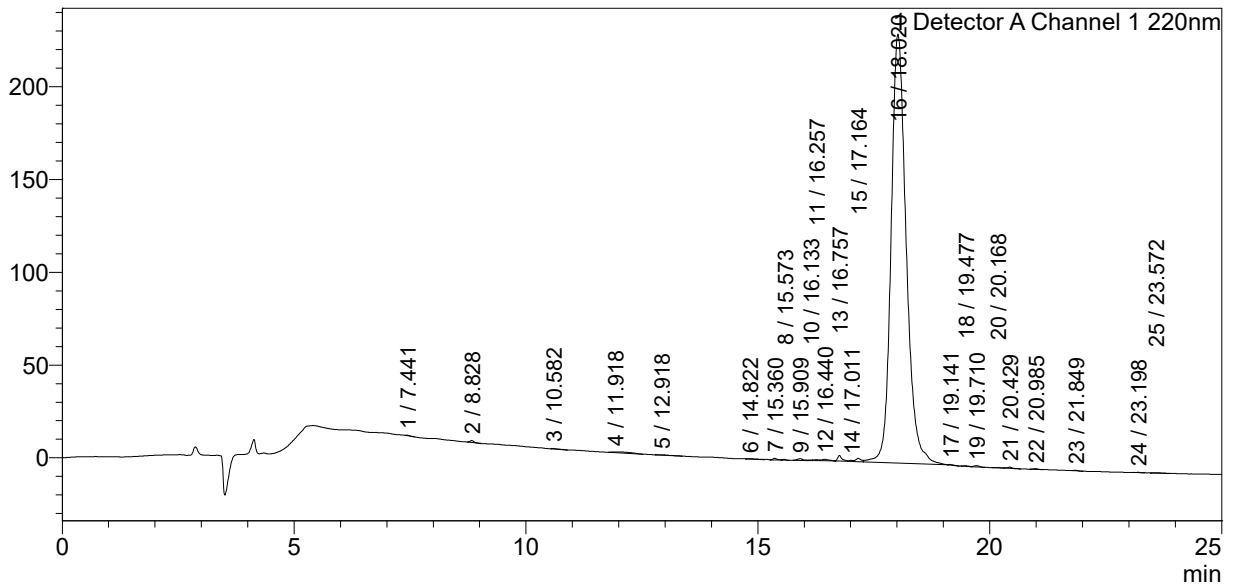

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.441	1059	267	0.020
2	8.828	5403	1016	0.101
3	10.582	1665	148	0.031
4	11.918	13606	340	0.254
5	12.918	2795	231	0.052
6	14.822	2042	153	0.038
7	15.360	4946	839	0.092
8	15.573	1563	388	0.029
9	15.909	8918	994	0.167
10	16.133	1779	316	0.033
11	16.257	4436	562	0.083
12	16.440	8467	831	0.158
13	16.757	20029	3059	0.374
14	17.011	3796	646	0.071
15	17.164	14817	1800	0.277
16	18.020	5231348	231121	97.812

Peak#	Ret. Time	Area	Height	Area%
17	19.141	1468	196	0.027
18	19.477	1988	280	0.037
19	19.710	4877	657	0.091
20	20.168	1032	153	0.019
21	20.429	4442	663	0.083
22	20.985	2565	399	0.048
23	21.849	1873	349	0.035
24	23.198	1404	239	0.026
25	23.572	2079	132	0.039
Total		5348397	245780	100.000