

Sample Name :OVA Peptide (323-339)
 Cat No. :RP10610
 Lot No. :E8213521C
 Time Processed :7:57:19
 Month-Day-Year Processed :03/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

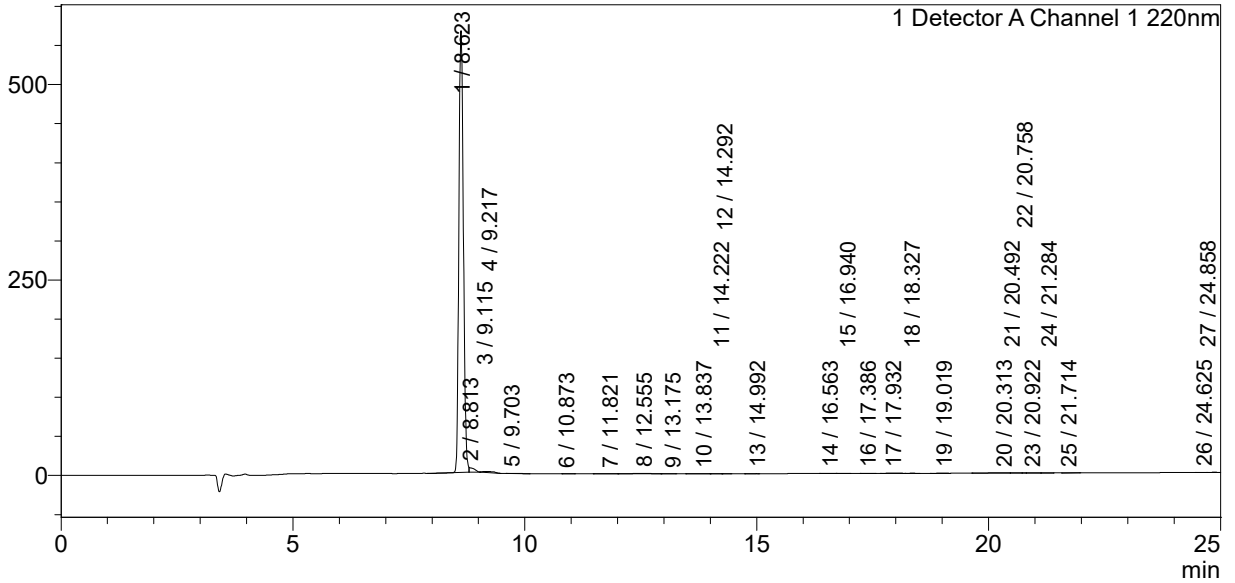

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.623	3812312	565291	96.056
2	8.813	43720	5942	1.102
3	9.115	5352	908	0.135
4	9.217	15995	1303	0.403
5	9.703	3726	253	0.094
6	10.873	1037	106	0.026
7	11.821	4358	193	0.110
8	12.555	18582	638	0.468
9	13.175	1858	136	0.047
10	13.837	2358	119	0.059
11	14.222	1267	109	0.032
12	14.292	1045	100	0.026
13	14.992	1558	104	0.039
14	16.563	2418	194	0.061

Peak#	Ret. Time	Area	Height	Area%
15	16.940	1131	101	0.028
16	17.386	1206	93	0.030
17	17.932	7866	416	0.198
18	18.327	1864	135	0.047
19	19.019	1494	120	0.038
20	20.313	18469	618	0.465
21	20.492	6211	465	0.156
22	20.758	1763	330	0.044
23	20.922	5056	331	0.127
24	21.284	2272	161	0.057
25	21.714	2737	199	0.069
26	24.625	1632	172	0.041
27	24.858	1561	132	0.039
Total		3968847	578669	100.000