

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : E7826921E
 Time Processed: 10:21:20
 Year-Month-Day: 2021/5/9

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	0	
5.00	Pumps	Solvent B Conc.	0	
20.00	Pumps	Solvent B Conc.	30	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
30.00	Pumps	Solvent B Conc.	95	
30.01	Pumps	Solvent B Conc.	0	
40.00	Pumps	Solvent B Conc.	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

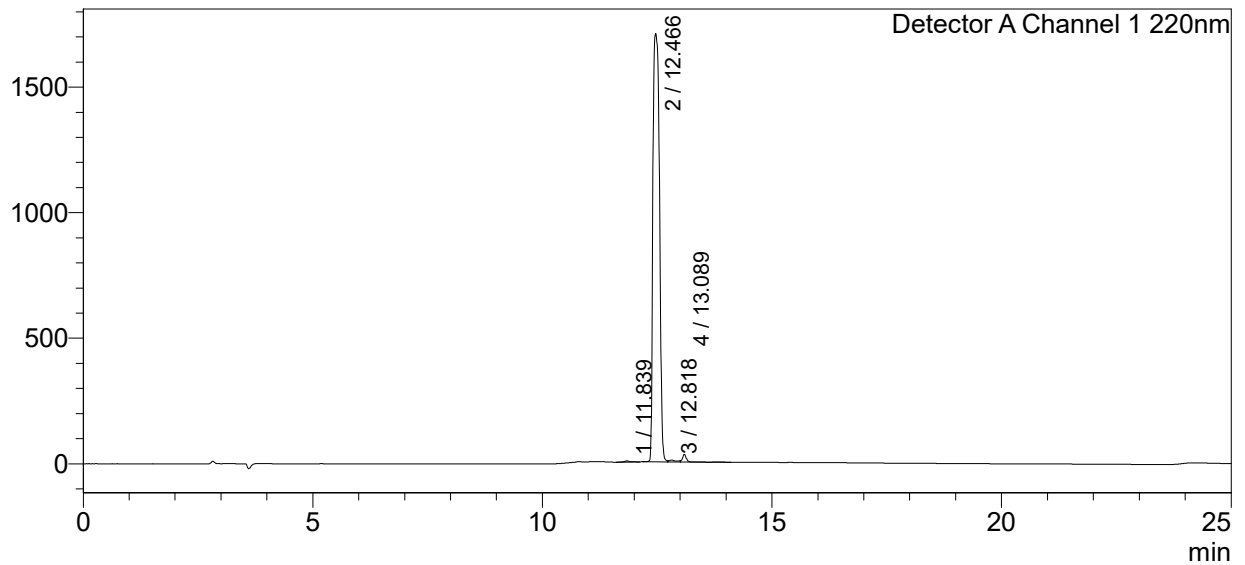

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.839	42375	4789	0.246
2	12.466	16906175	1706867	98.021
3	12.818	87693	7985	0.508
4	13.089	211268	31336	1.225
Total		17247511	1750977	100.000