

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : E7250321A
 Month-Day-Year Processed : 01/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

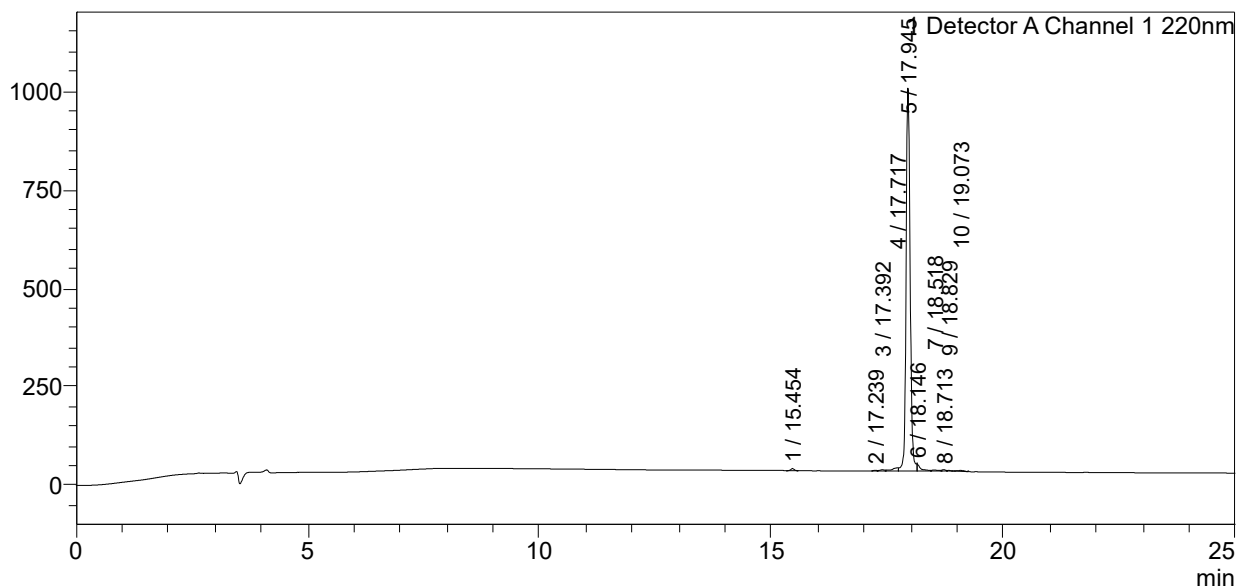

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.454	26443	5317	0.427
2	17.239	7287	1374	0.118
3	17.392	22505	2806	0.364
4	17.717	71134	8013	1.149
5	17.945	5889105	970984	95.156
6	18.146	93979	17562	1.519
7	18.518	25114	2965	0.406
8	18.713	22610	3749	0.365
9	18.829	7351	1647	0.119
10	19.073	23393	2328	0.378
Total		6188921	1016745	100.000