

Sample Name : Influenza A NP(366-374) Strain A/PR/8/35  
 Cat. No. : RP20267  
 Lot. No. : PE8731902  
 Time Processed : 9:09:28  
 Month-Day-Year Processed : 03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

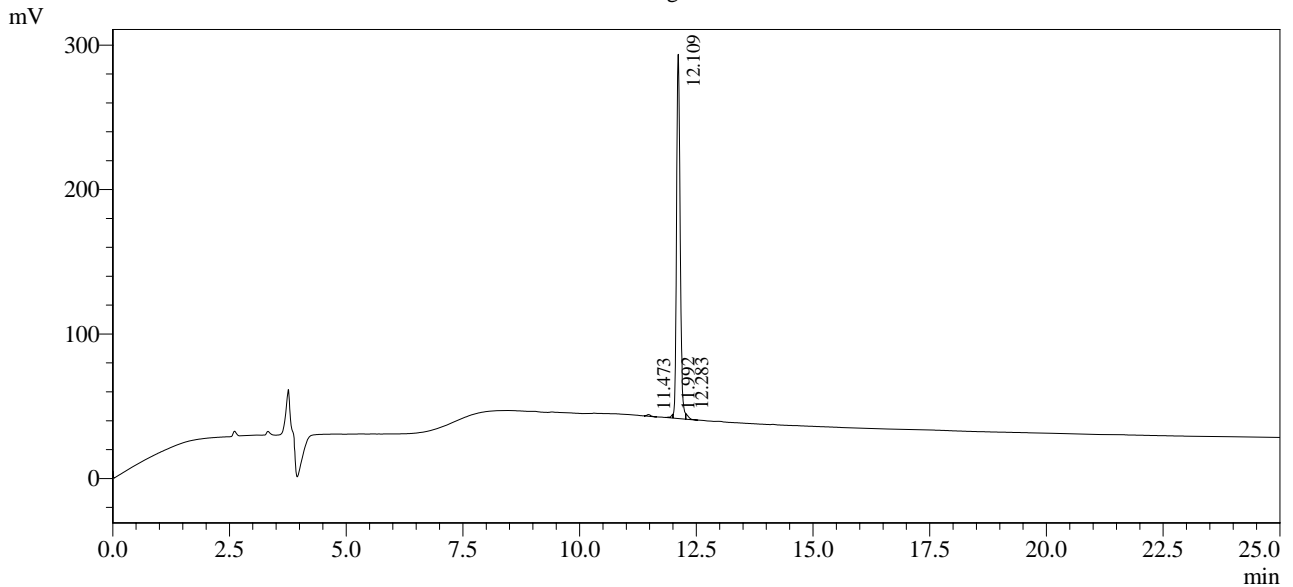

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.473	6341	1188	0.455
2	11.992	8293	2499	0.596
3	12.109	1364892	251810	98.020
4	12.283	12933	3568	0.929
Total		1392459	259065	100.000