

Sample Name : α -MSH, amide
 Cat. No.: RP10644
 Lot. No. :PE8991811
 Time Processed :14:50:11
 Month-Day-Year Processed :11/29/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

Chromatogram

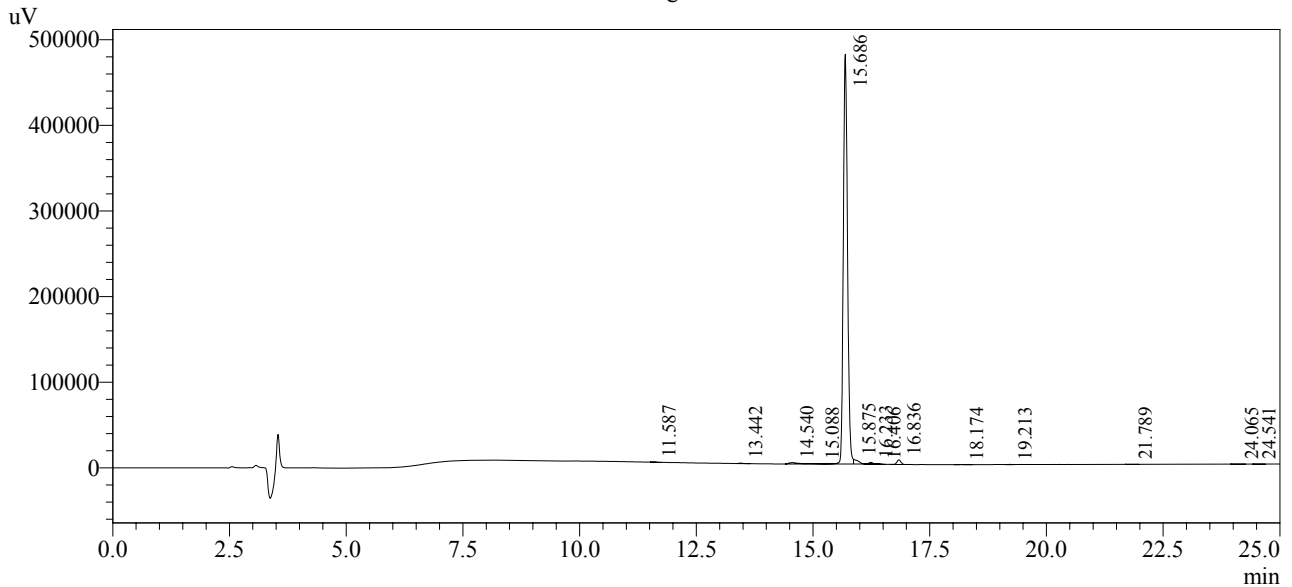

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.587	1930	351	0.062
2	13.442	3603	582	0.116
3	14.540	27966	1717	0.900
4	15.088	3528	331	0.114
5	15.686	2976283	478639	95.785
6	15.875	38206	5309	1.230
7	16.233	11174	1964	0.360
8	16.406	1785	343	0.057
9	16.836	32185	5385	1.036
10	18.174	1950	179	0.063
11	19.213	1894	223	0.061
12	21.789	1957	180	0.063
13	24.065	2421	247	0.078
14	24.541	2383	271	0.077
Total		3107266	495719	100.000