

Sample Name :Palmitoyl Tetrapeptide-3
 Sample ID :U6182GA220-1
 Time Processed :9:08:48
 Month-Day-Year Processed :01/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

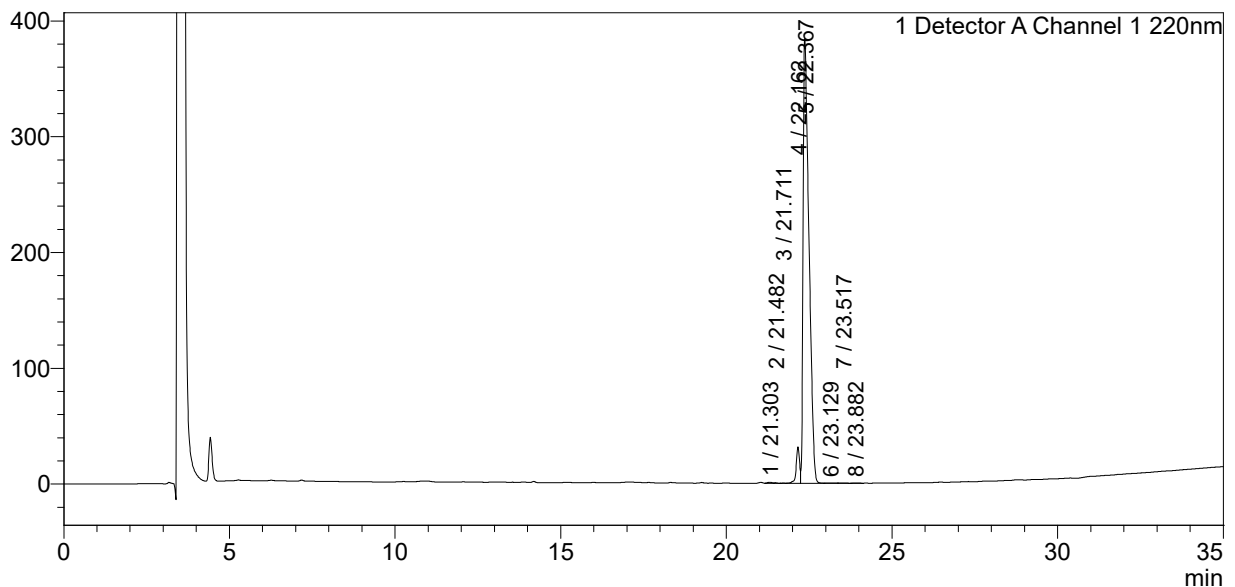

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.303	9081	938	0.183
2	21.482	2687	413	0.054
3	21.711	1163	157	0.023
4	22.162	221810	31351	4.459
5	22.367	4729111	384147	95.069
6	23.129	5029	297	0.101
7	23.517	3314	231	0.067
8	23.882	2178	200	0.044
Total		4974373	417734	100.000