

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No. : RP11095  
 Lot No. : E3965820K  
 Time Processed : 9:03:32  
 Month-Day-Year Processed : 11/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : ZJ19010141

<Chromatogram>

mV

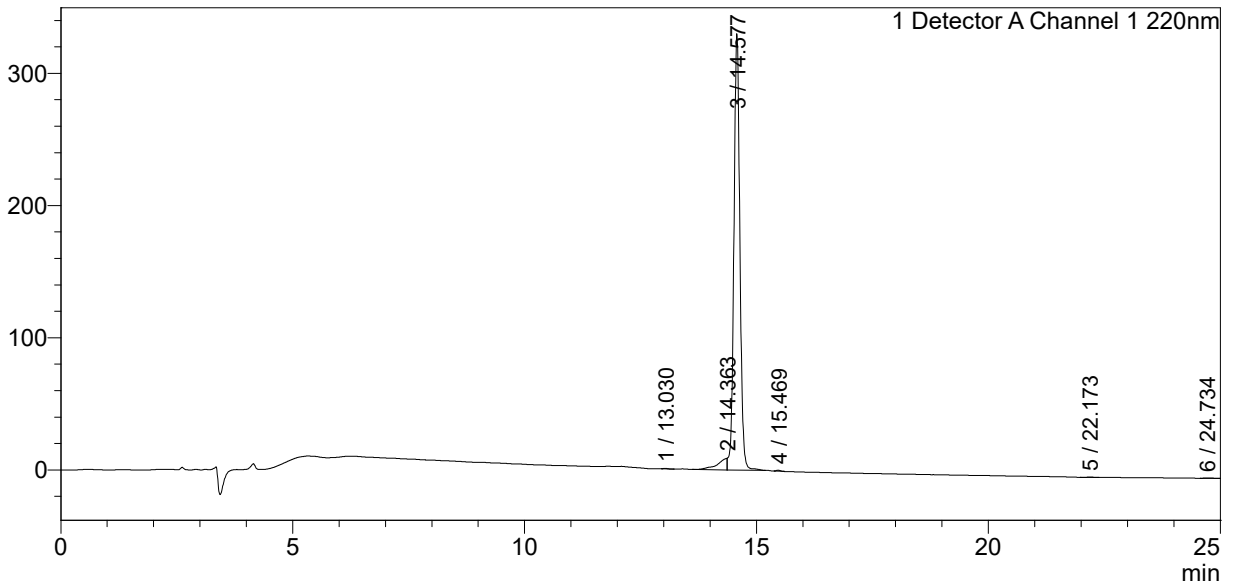

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.030	2374	398	0.077
2	14.363	125942	8728	4.073
3	14.577	2955745	330173	95.584
4	15.469	4578	781	0.148
5	22.173	1060	78	0.034
6	24.734	2587	211	0.084
Total		3092286	340369	100.000