

Sample Name :β-Amyloid (25-35)  
 Cat. No. : RP10008  
 Lot. No. : PE9981806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


| Time  | Unit       | Command       | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01  | Pumps      | Pump A B.Conc | 5     |         |
| 25.00 | Pumps      | Pump A B.Conc | 65    |         |
| 25.01 | Pumps      | Pump A B.Conc | 95    |         |
| 27.00 | Pumps      | Pump A B.Conc | 95    |         |
| 27.01 | Pumps      | Pump A B.Conc | 5     |         |
| 35.00 | Pumps      | Pump A B.Conc | 5     |         |
| 35.01 | Controller | Stop          |       |         |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

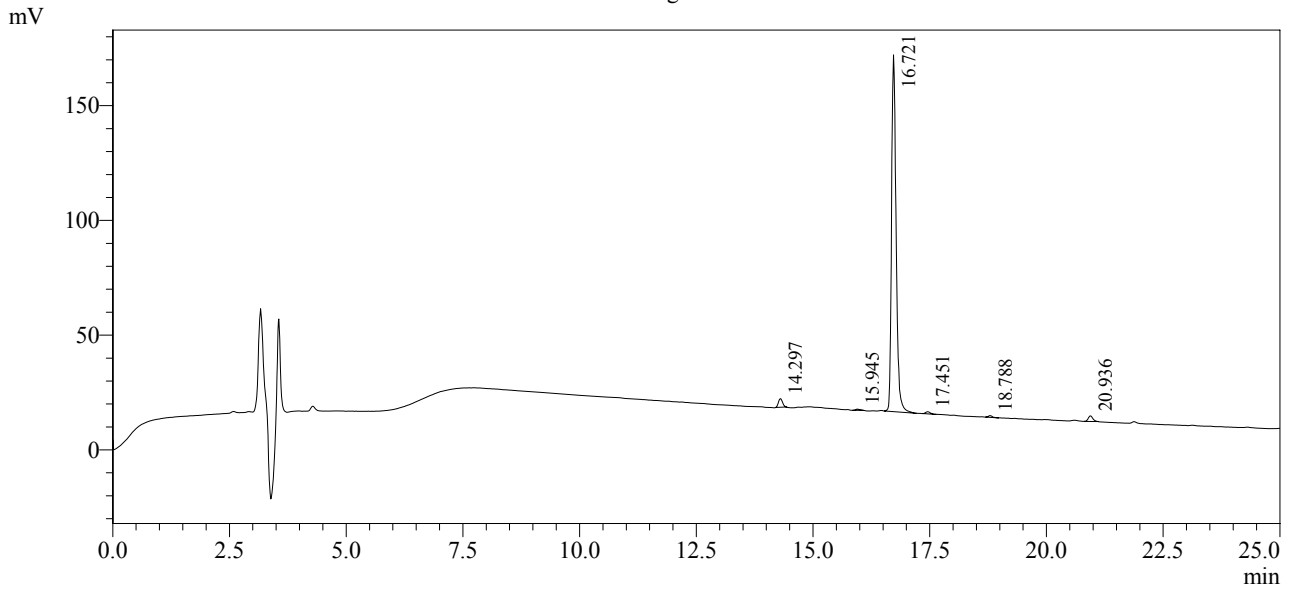

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area    | Height | Area %  |
|-------|-----------|---------|--------|---------|
| 1     | 14.297    | 23211   | 3802   | 2.083   |
| 2     | 15.945    | 3407    | 513    | 0.306   |
| 3     | 16.721    | 1060753 | 155495 | 95.214  |
| 4     | 17.451    | 6180    | 919    | 0.555   |
| 5     | 18.788    | 4244    | 743    | 0.381   |
| 6     | 20.936    | 16283   | 2418   | 1.462   |
| Total |           | 1114078 | 163890 | 100.000 |