

Sample Name :Cortistatin 14, human, rat
 Cat. No. : RP10972
 Lot. No.: PE2011905
 Time Processed : 14:01:30
 Month-Day-Year Processed : 06/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
45.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

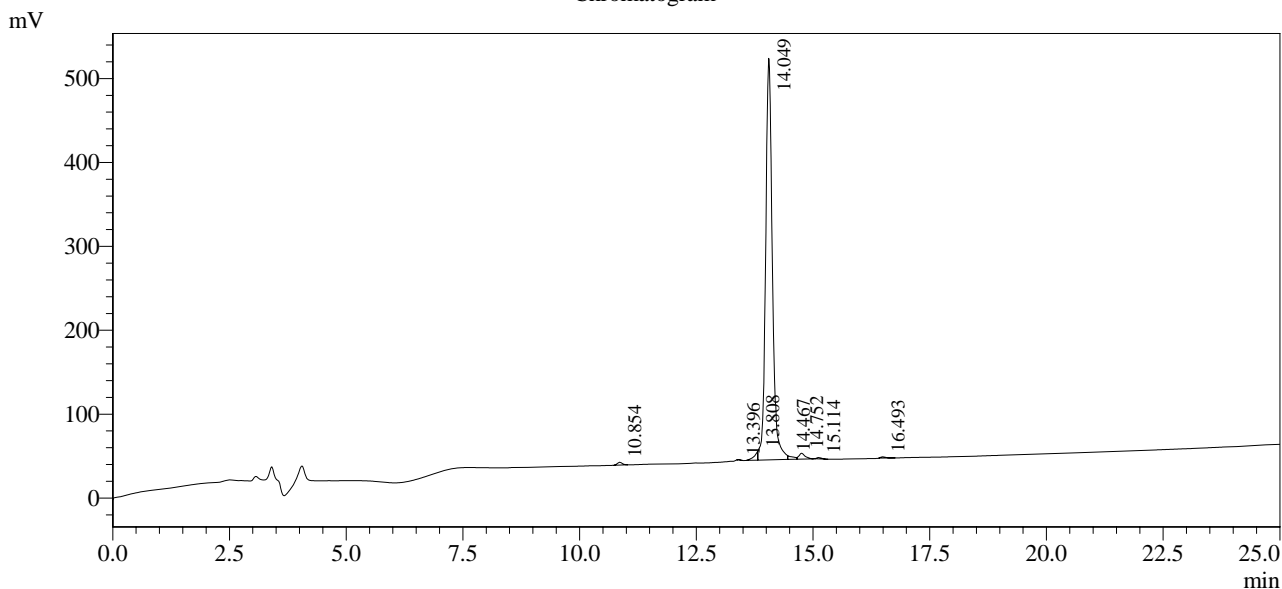

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.854	24077	3294	0.484
2	13.396	2426	637	0.049
3	13.808	55549	10082	1.116
4	14.049	4772393	478703	95.897
5	14.467	34980	4288	0.703
6	14.752	64125	7016	1.289
7	15.114	12187	1644	0.245
8	16.493	10822	1514	0.217
Total		4976558	507178	100.000