


Mass Spectrum

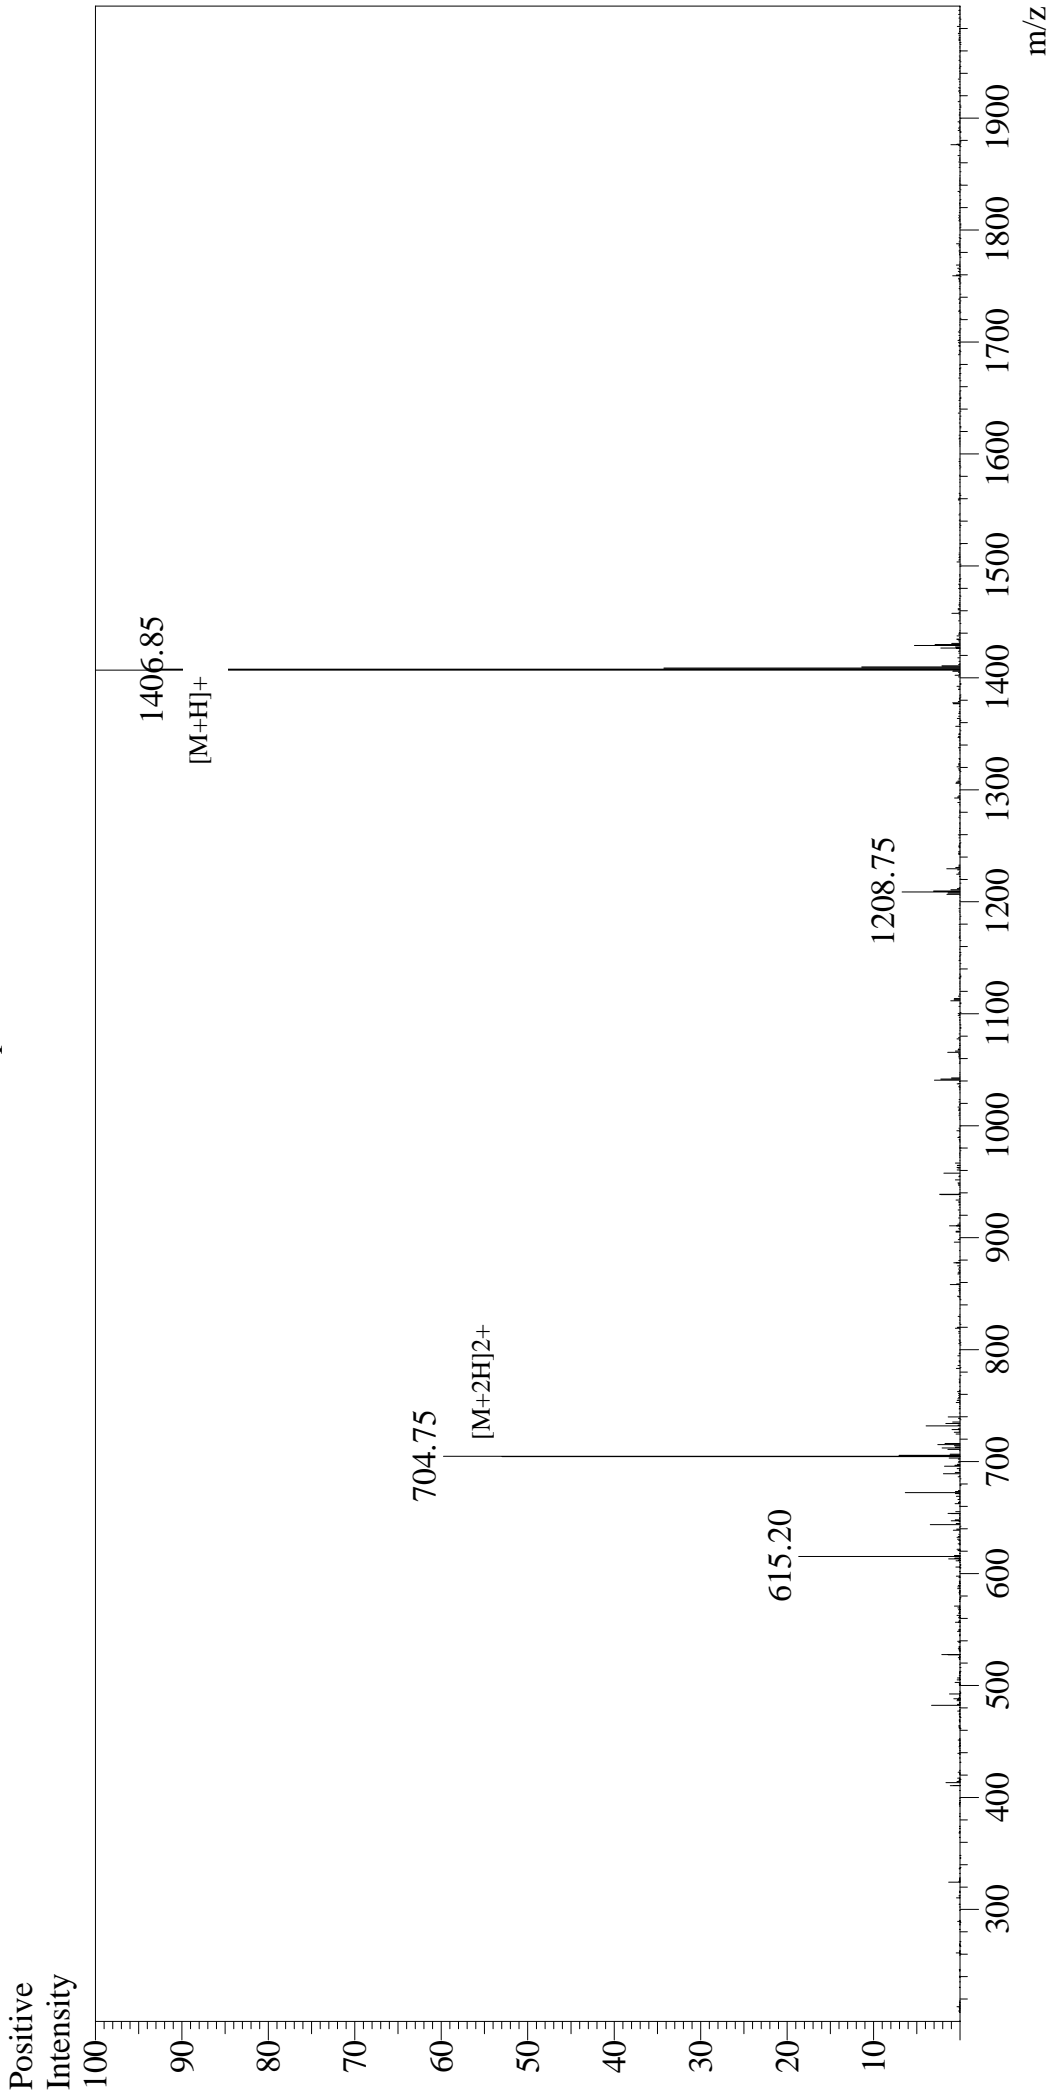

Sample Information

User : Gary
Month-Day Processed : 07/20/17
Time Processed : 15:35:13
Injection Volume : 0.2
Sample Name : Hepatitis B Virus Core (128-140)
Cat No. : RP17313
Lot No. : PE4121707
Theoretical MW : 1406.63
Observed MW : 1405.85

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250 °C
Block Temp : 200 °C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH