

Sample Name:β-Endorphin, human

Cat. No. : RP11344

Lot. No. : E6521420B

Time Processed: 15:33:14

Month-Day-Year Processed :02/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Equipment:ZJ19010324

<Chromatogram>

mV

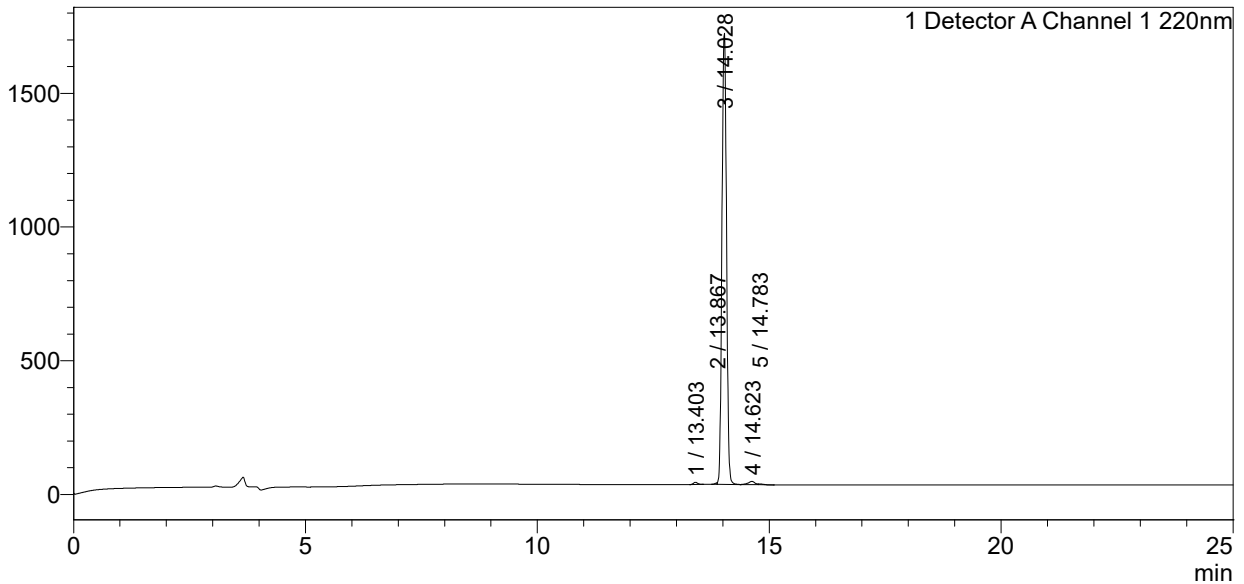

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.403	48268	7852	0.411
2	13.867	17058	5076	0.145
3	14.028	11528246	1687763	98.202
4	14.623	122674	12228	1.045
5	14.783	23083	3083	0.197
Total		11739330	1716003	100.000