

Sample Name :Parathyroid Hormone (PTH) (1-34), Human
 Cat No.: RP01001
 Lot No.: E3953320D
 Time Processed :2:56:03
 Month-Day-Year Processed :04/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

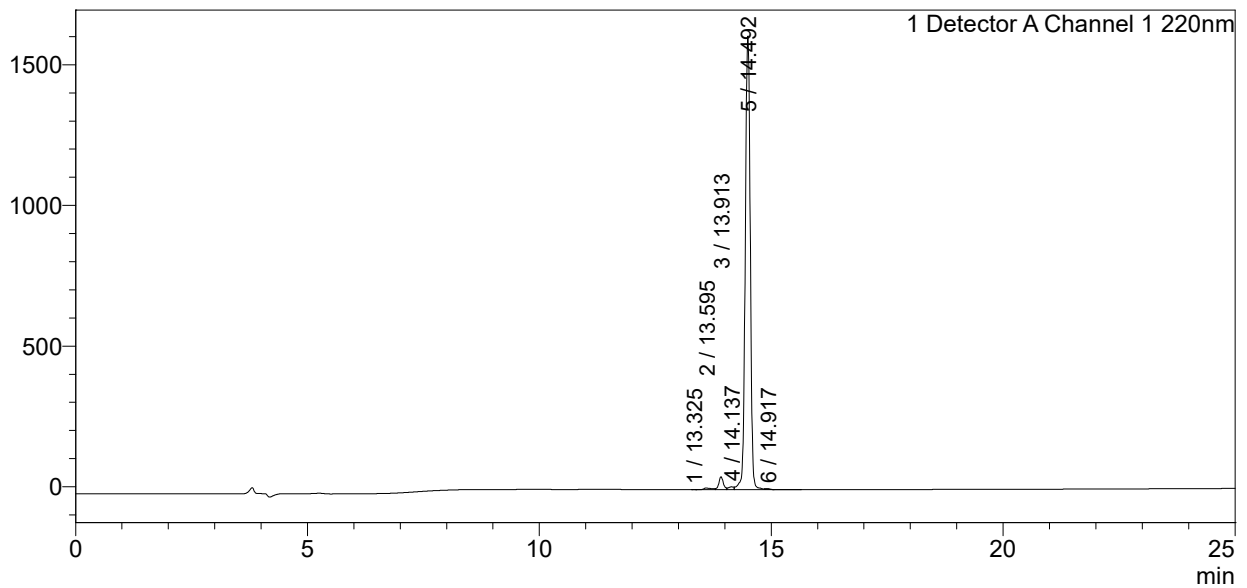

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.325	243	57	0.002
2	13.595	72443	5866	0.576
3	13.913	311779	46077	2.478
4	14.137	80929	10042	0.643
5	14.492	12107661	1612999	96.212
6	14.917	11288	2189	0.090
Total		12584343	1677230	100.000