

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : E4945620I
 Time Processed : 3:19:51
 Month-Day-Year Processed : 09/30/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	60
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010324

<Chromatogram>

mV

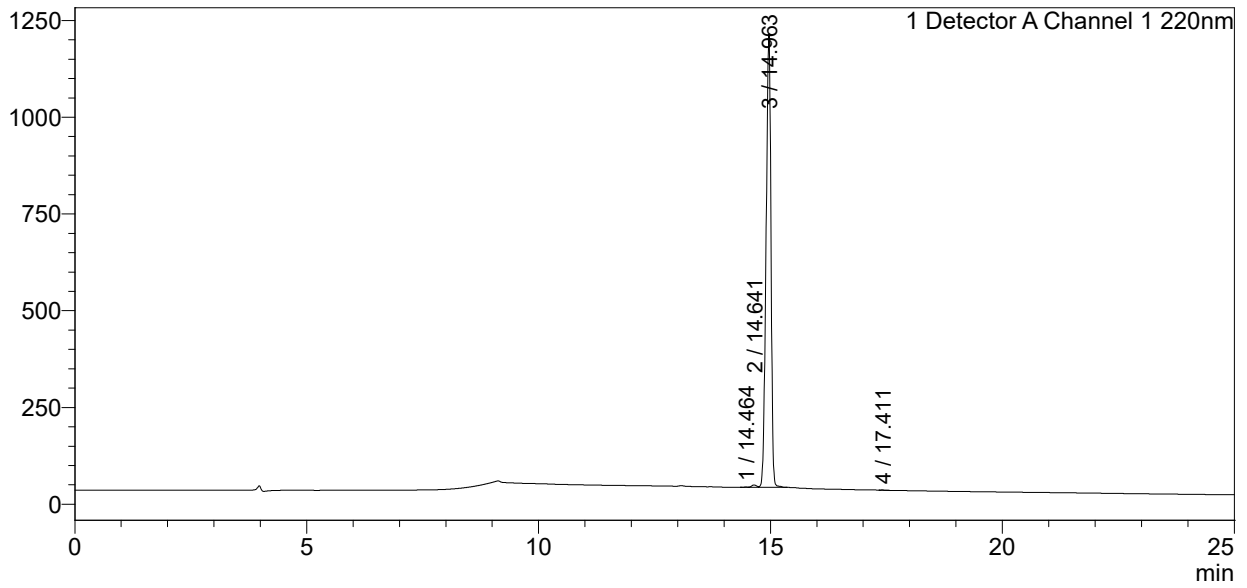

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.464	5046	822	0.058
2	14.641	48869	6352	0.566
3	14.963	8570699	1172767	99.341
4	17.411	2902	554	0.034
Total		8627516	1180495	100.000