


Mass Spectrum

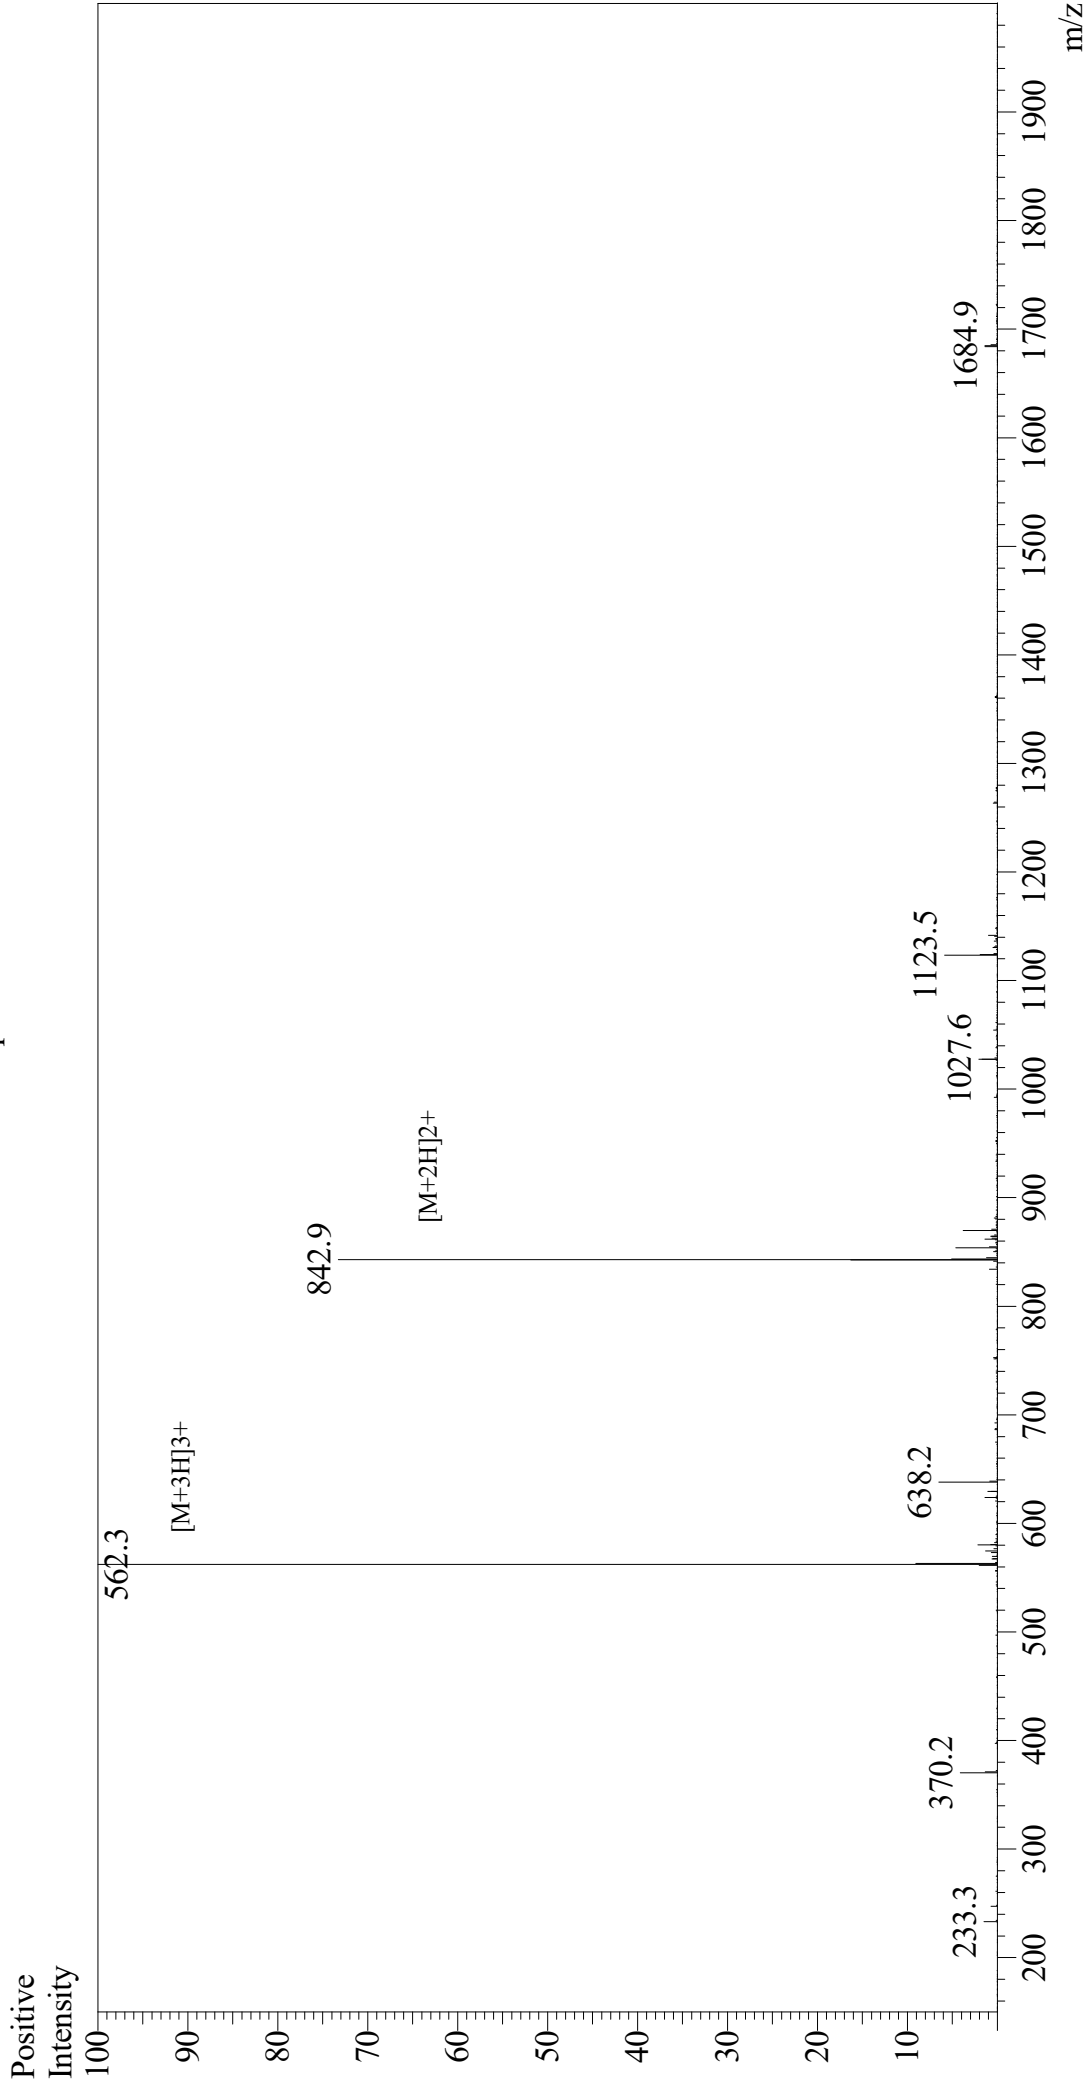

Sample Information
Month-Day Processed : 07/24/21
Time Processed : 21:05:58
Injection Volume : 0.2
Sample Name : α -Factor Mating Pheromone, yeast
Cat. No. : RP01002
Lot. No. : E6109421G
Theoretical MW : 1683.98
Observed MW : 1683.9

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH