

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : PE0221903
 Time Processed : 22:34:09
 Month-Day-Year Processed : 03/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

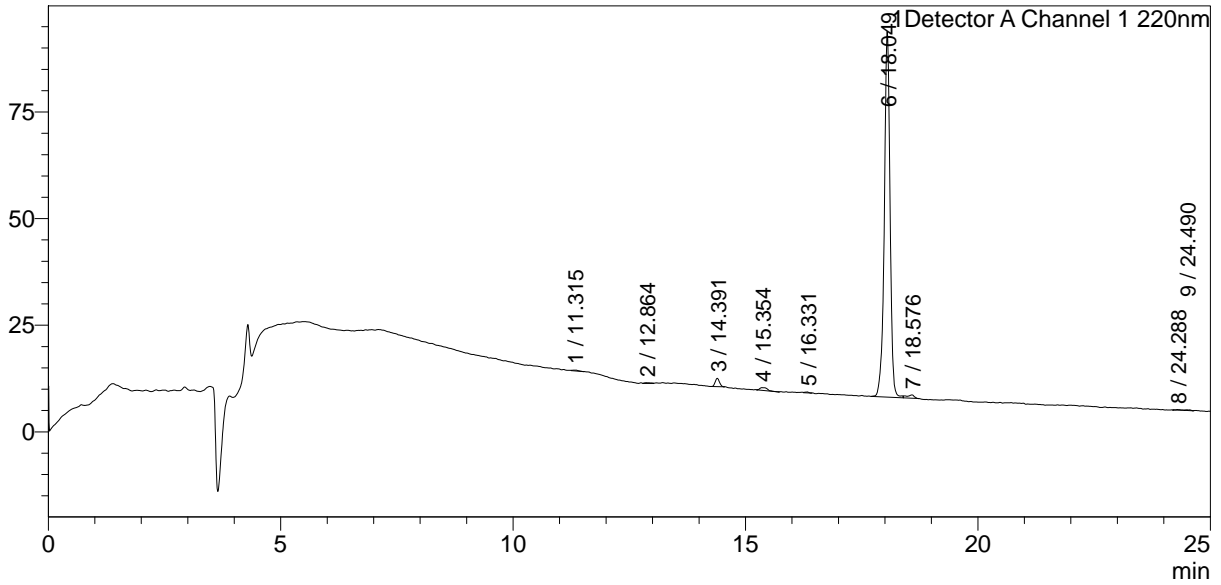

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.315	1657	169	0.216
2	12.864	1600	162	0.208
3	14.391	12438	1951	1.618
4	15.354	7302	635	0.950
5	16.331	1154	210	0.150
6	18.049	733969	85726	95.475
7	18.576	8571	784	1.115
8	24.288	1022	135	0.133
9	24.490	1045	136	0.136
Total		768759	89908	100.000