

Sample Name :Melittin,honey bee
 Cat. No. : RP20415
 Lot. No. : PE7571902
 Month-Day-Year Processed : 03/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

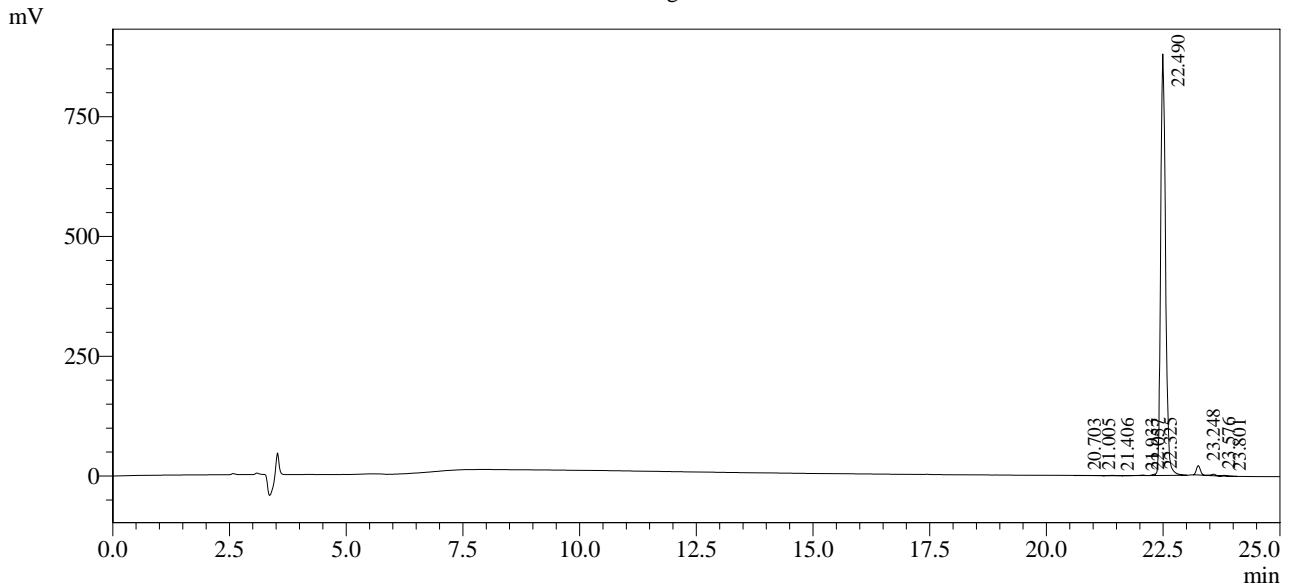

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	20.703	5258	797	0.080
2	21.005	5239	847	0.079
3	21.406	5007	619	0.076
4	21.933	3599	368	0.054
5	22.057	6100	931	0.092
6	22.325	12698	2778	0.192
7	22.490	6419278	879877	97.168
8	23.248	114980	19395	1.740
9	23.576	24553	3177	0.372
10	23.801	9644	1614	0.146
Total		6606356	910403	100.000