


Mass Spectrum

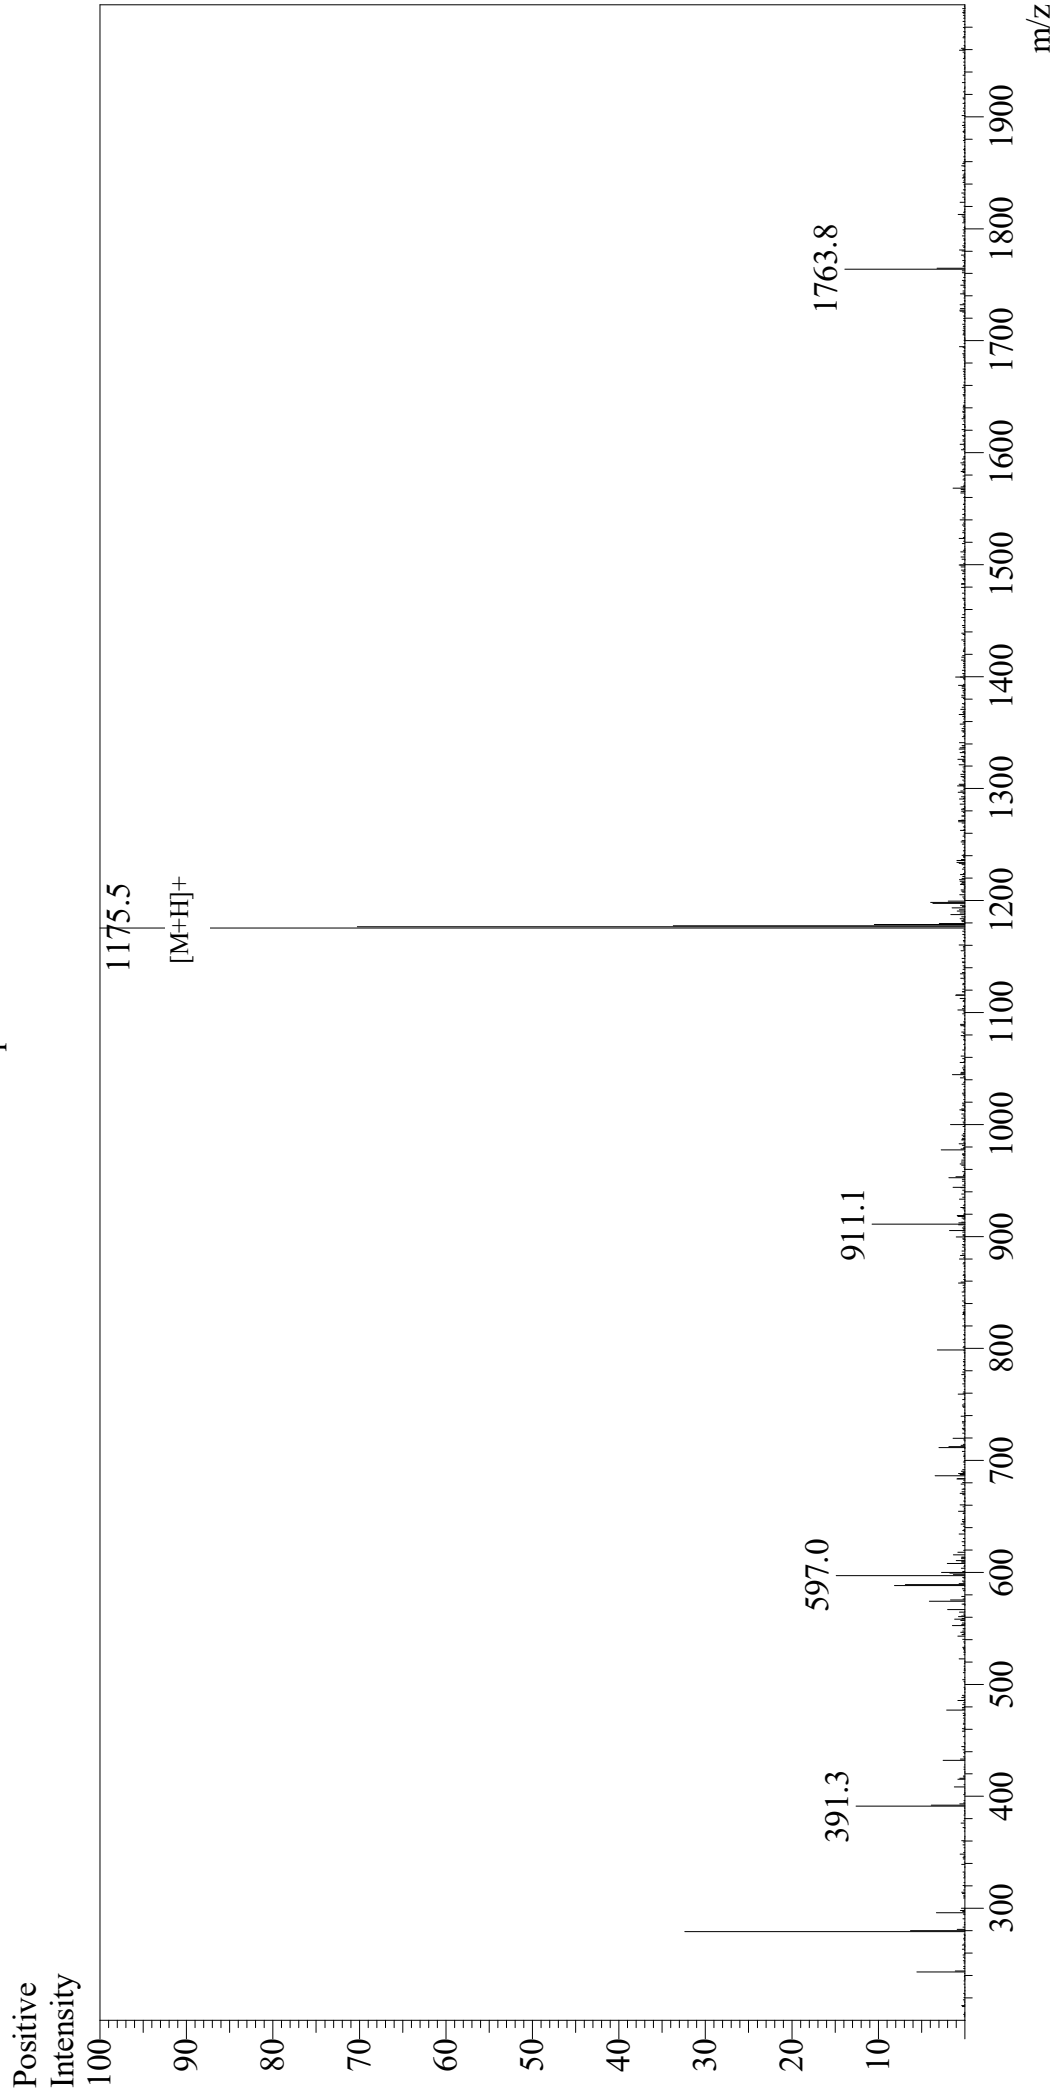

Sample Information

User : Gary
Month-Day Processed : 11/09/19
Time Processed : 02:57:30 PM
Injection Volume : 0.3
Sample Name : mTRP-2(180-188)
Cat No. : RP20250
Lot No. : E7534919K
Theoretical MW : 1175.34
Observed MW : 1174.5

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH