

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : PE7891812
 Time Processed : 10:11:02
 Month-Day-Year Processed : 12/24/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
32.00	Pumps	Pump B Conc.	95	
32.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

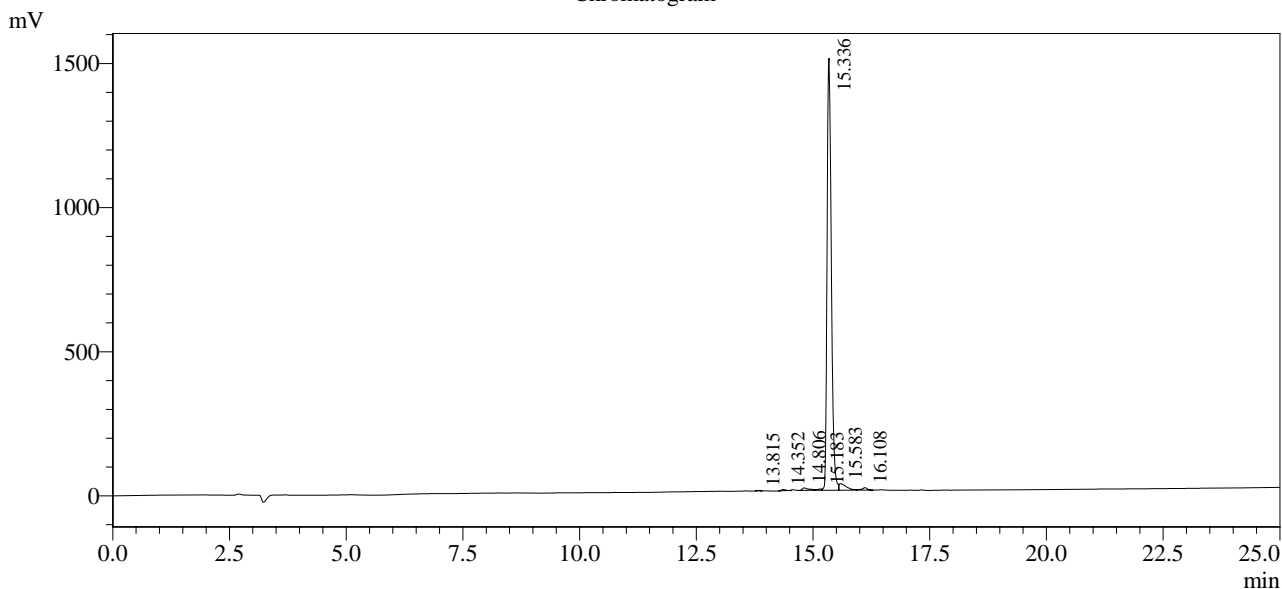

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.815	7351	1814	0.073
2	14.352	24865	4432	0.248
3	14.806	81558	8617	0.813
4	15.183	32451	4664	0.324
5	15.336	9571176	1498756	95.449
6	15.583	245464	22592	2.448
7	16.108	64680	8475	0.645
Total		10027545	1549348	100.000