

Sample Name :  $\beta$ -Amyloid (1-40)  
 Cat. No. : RP10004  
 Lot. No. : PE6771710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

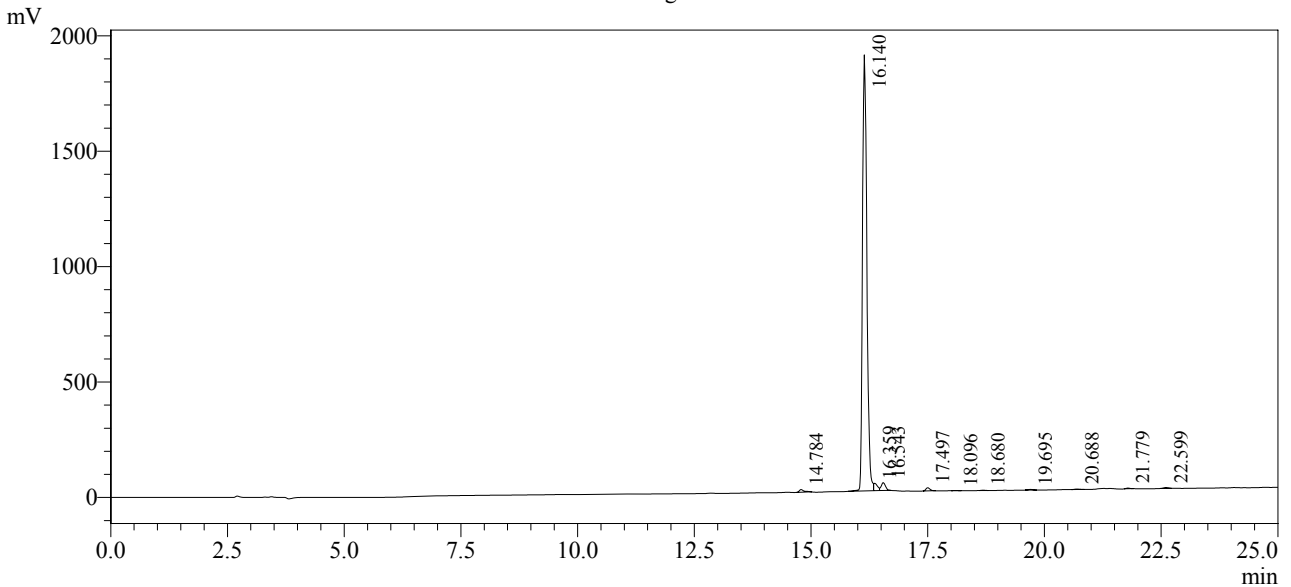

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.784	86198	11628	0.664
2	16.140	12344602	1889191	95.110
3	16.359	170213	31787	1.311
4	16.543	214225	33992	1.651
5	17.497	82803	13647	0.638
6	18.096	6117	1010	0.047
7	18.680	6837	1242	0.053
8	19.695	17363	2642	0.134
9	20.688	13622	1812	0.105
10	21.779	16519	2998	0.127
11	22.599	20851	3083	0.161
Total		12979351	1993031	100.000