


Mass Spectrum

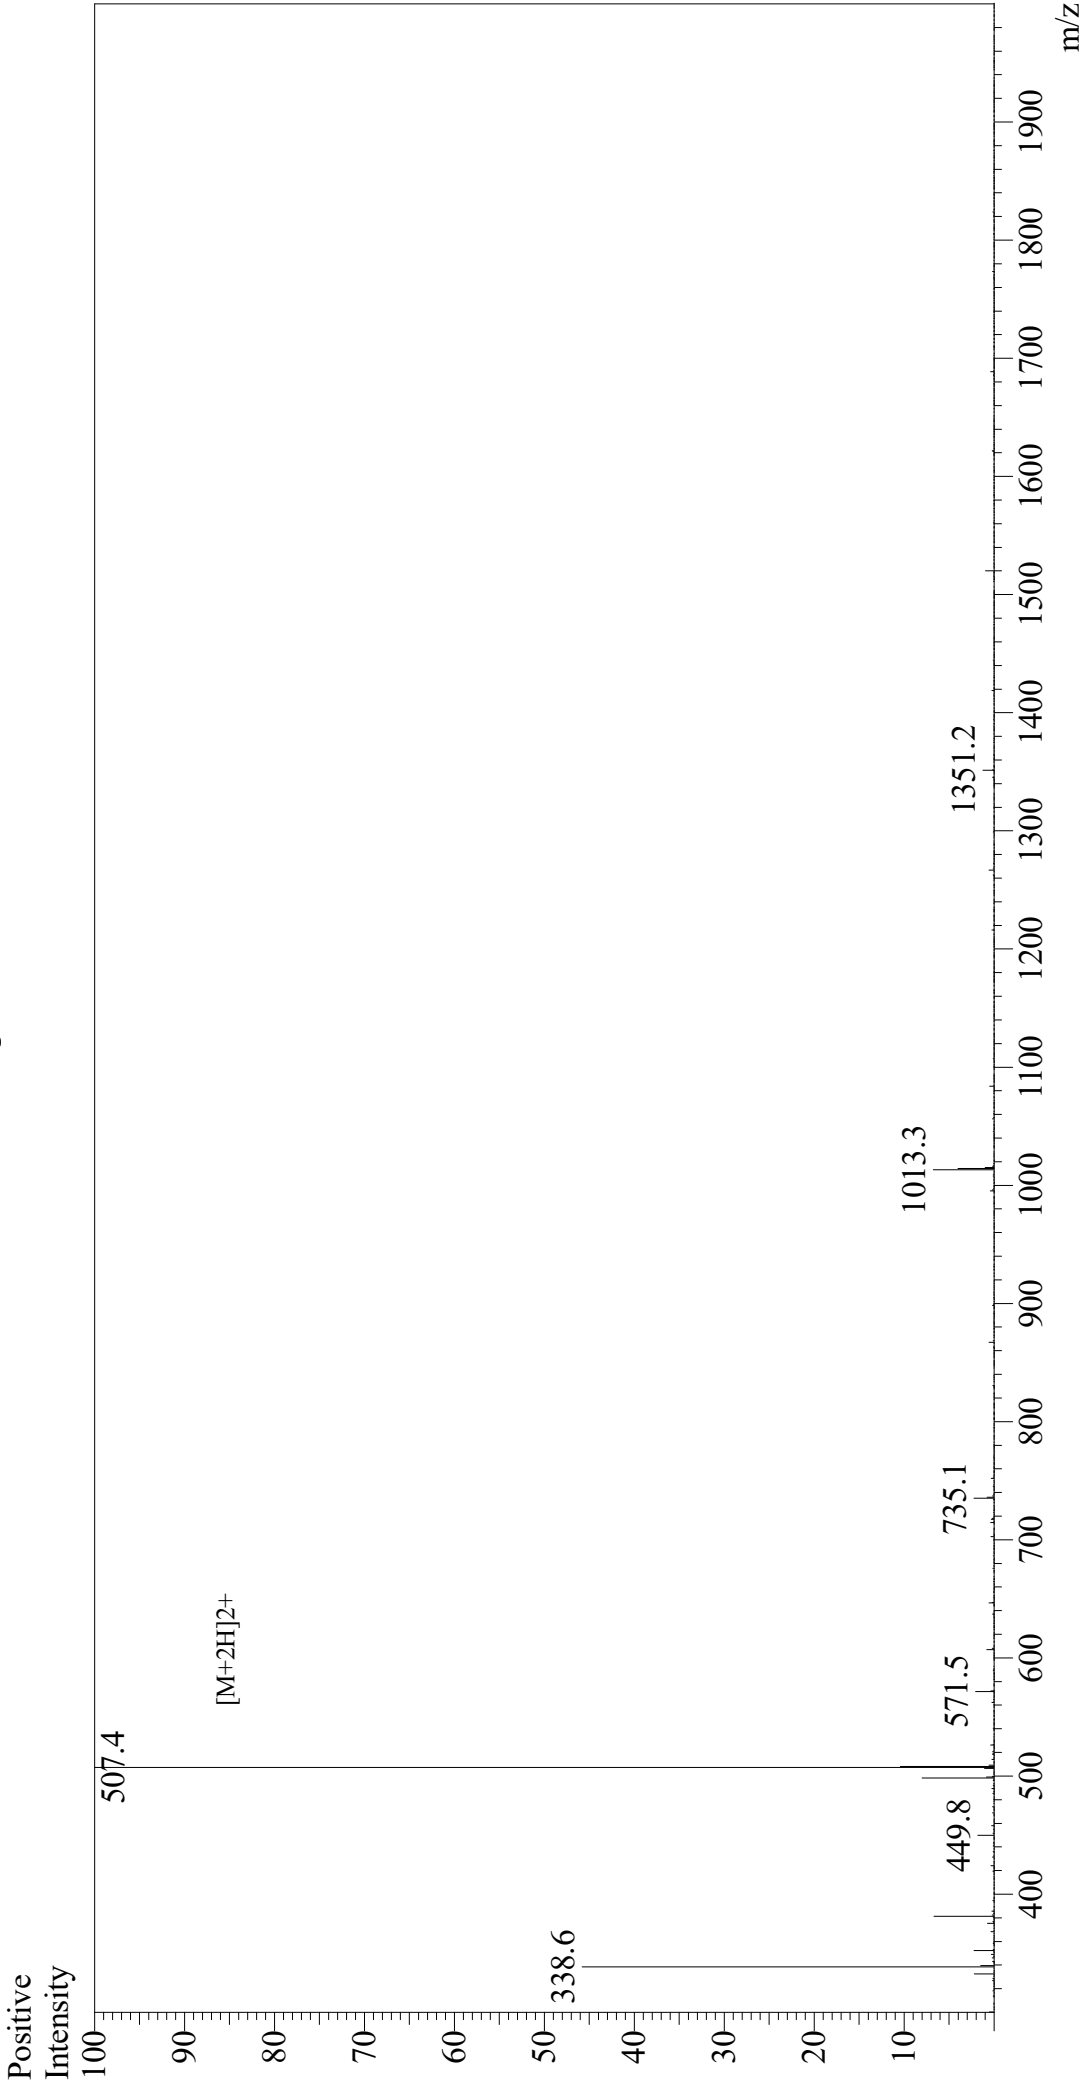

Sample Information

Acquired by : Gary

Month-Day Processed : 05/13/20

Time Processed : 02:42:49 PM

Injection Volume : 0.3

Sample Name : DYKDDDDK Peptide

Cat No. : RP10586

Lot No. : E9824020E

Theoretical MW : 1012.97

Observed MW : 1012.8

Equipment : GK11010007

Interface Bias : +4.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50% H₂O/50% MeOH

Interface : ESI

Nebulizing Gas Flow : 1.5 L/min

CDL Temp : 250

Block Temp : 200

1351.2