

Sample Name: C-Myc Peptide  
 Cat No. : RP11731  
 Lot No. : E3991221F  
 Time Processed : 22:48:48  
 Month-Day-Year Processed : 06/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

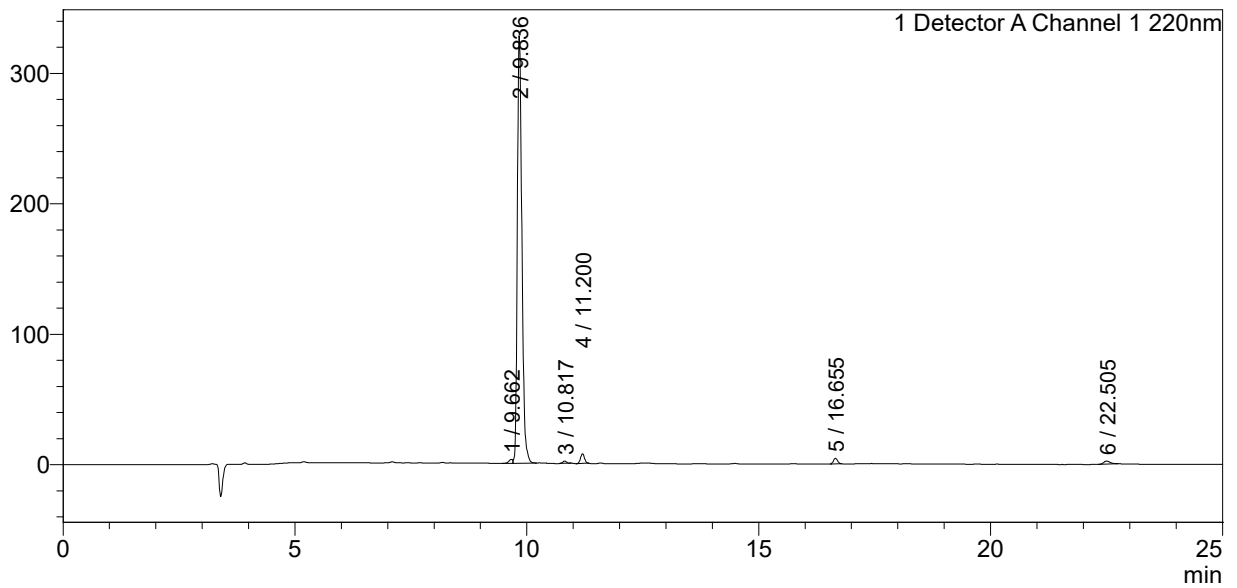

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.662	17990	3033	0.760
2	9.836	2248073	327814	95.006
3	10.817	9661	1730	0.408
4	11.200	43041	7360	1.819
5	16.655	25330	4151	1.070
6	22.505	22147	2353	0.936
Total		2366242	346440	100.000