

Sample Name :IRBP (1-20), human
 Cat. No. :RP20269
 Lot. No. :PE8021802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

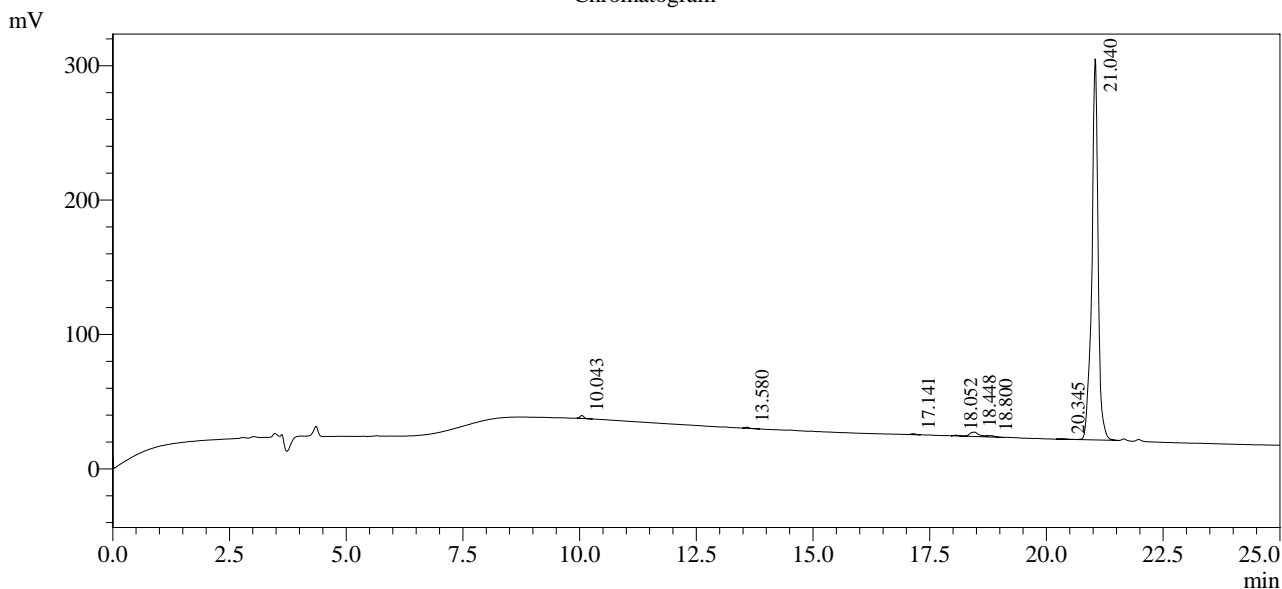

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.043	13079	2276	0.478
2	13.580	4338	796	0.158
3	17.141	4844	762	0.177
4	18.052	4031	547	0.147
5	18.448	45581	3238	1.665
6	18.800	10674	1081	0.390
7	20.345	3760	326	0.137
8	21.040	2651296	283611	96.847
Total		2737603	292636	100.000