


Mass Spectrum

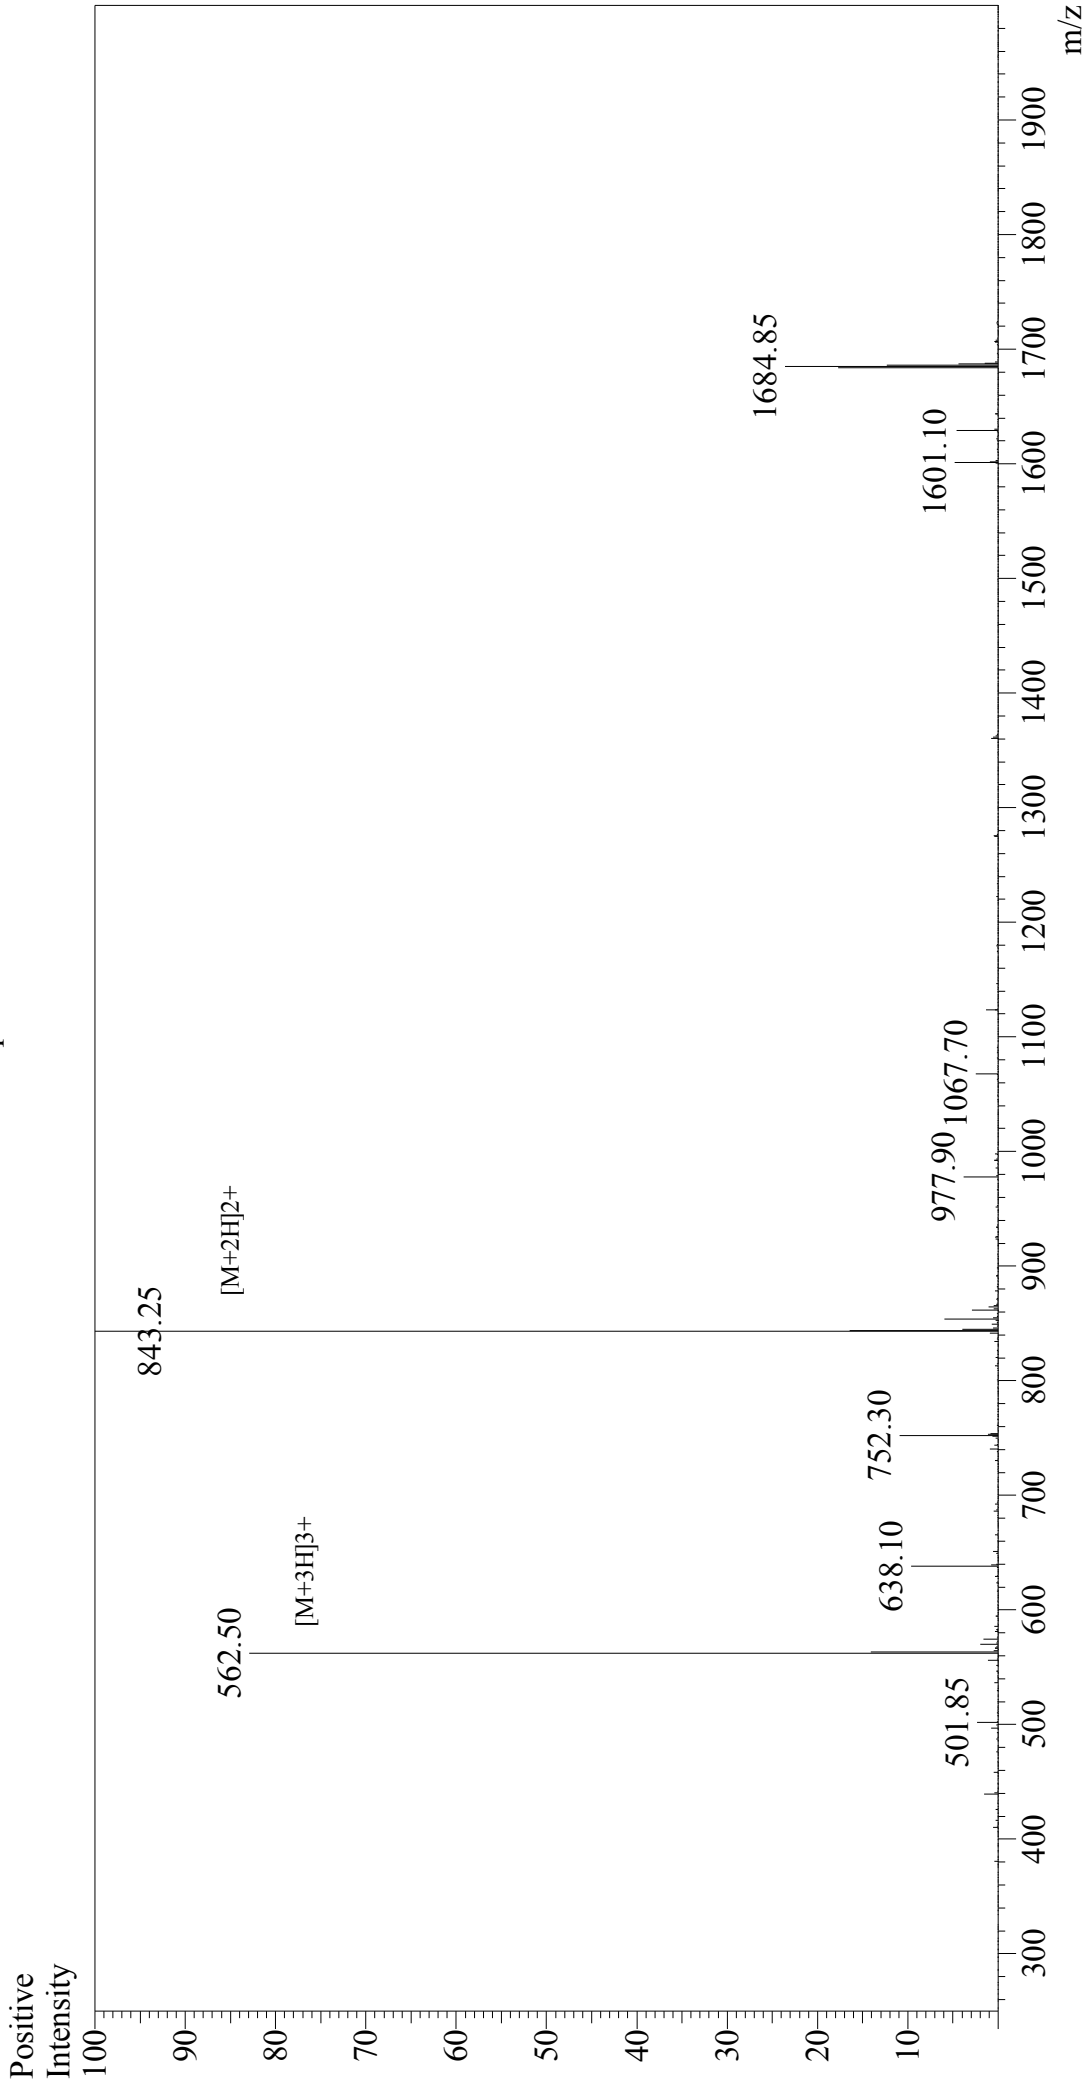

Sample Information

Acquired by : Gary
Month-Day Processed : 10/04/17
Time Processed : 9:28:36
Injection Volume : 0.2
Sample Name : α -Factor Mating Pheromone, yeast
Cat. No : RP01002
Lot. No : PE2151708
Theoretical MW : 1683.98
Observed MW : 1684.50

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH