

Sample Name :GRGDSPC
 Cat. No. : RP20283
 Lot. No. :E4870519I
 Time Processed :16:32:59
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

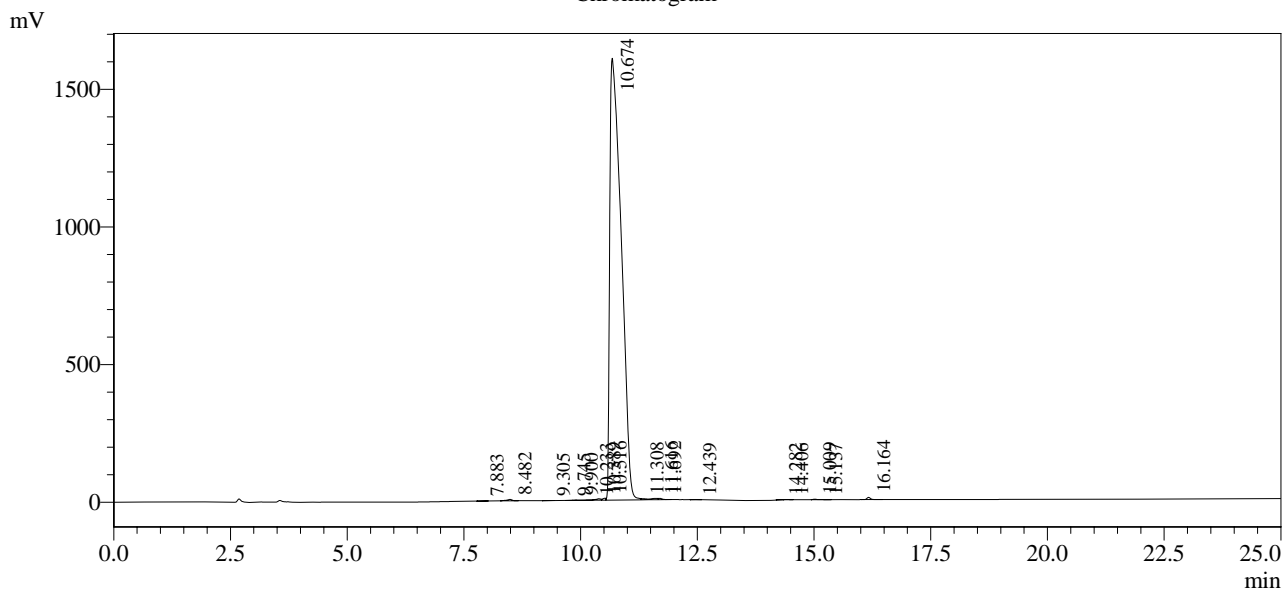

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.883	2733	393	0.010
2	8.482	38984	4899	0.141
3	9.305	4189	608	0.015
4	9.745	3080	501	0.011
5	9.900	6837	1047	0.025
6	10.233	11323	894	0.041
7	10.389	42566	5292	0.154
8	10.516	31300	6774	0.113
9	10.674	27325996	1605194	98.876
10	11.308	33824	4134	0.122
11	11.616	49673	4725	0.180
12	11.692	25001	4609	0.090
13	12.439	1042	238	0.004
14	14.282	691	155	0.002
15	14.406	3339	620	0.012
16	15.009	9324	1773	0.034
17	15.137	2345	431	0.008
18	16.164	44396	8167	0.161
Total		27636642	1650453	100.000