

Sample Name :Hexa-His  
 Cat No.: RP11737  
 Lot No.: E4978120B  
 Time Processed :9:12:19  
 Month-Day-Year Processed :02/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

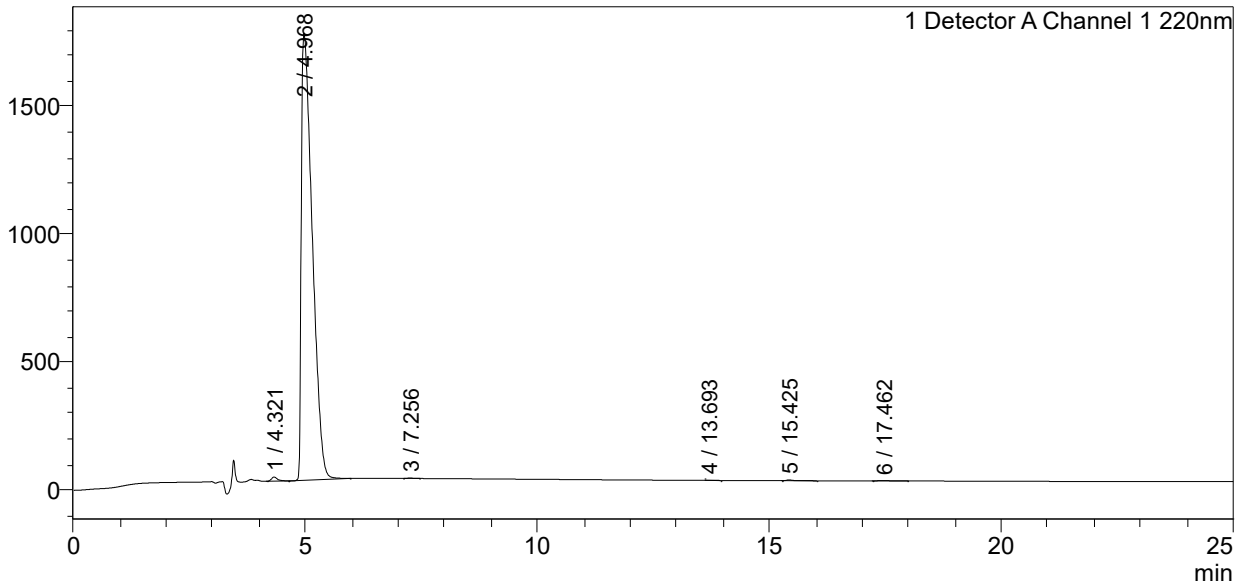

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.321	152164	16373	0.526
2	4.968	28719103	1747691	99.226
3	7.256	12266	2053	0.042
4	13.693	1922	344	0.007
5	15.425	29908	3217	0.103
6	17.462	27632	1767	0.095
Total		28942995	1771444	100.000