

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No :RP11529
 Lot No :E2605121A
 Time Processed :2:25:24 PM
 Month-Day-Year Processed :01/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

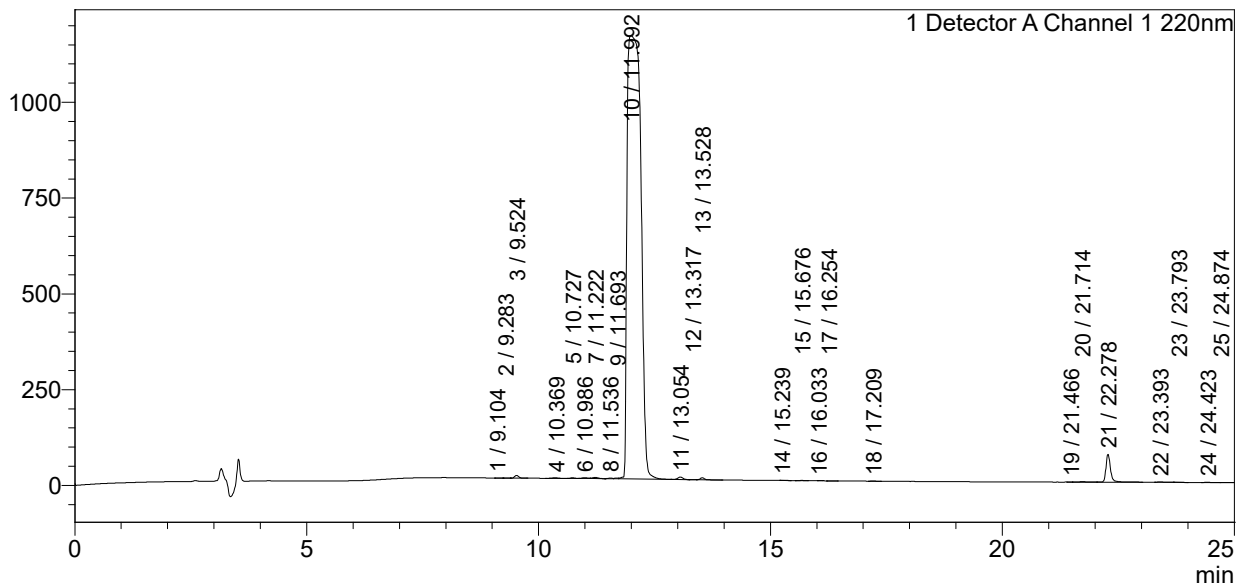

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.104	2255	229	0.009
2	9.283	1879	333	0.008
3	9.524	44005	7249	0.180
4	10.369	13081	1410	0.054
5	10.727	11432	1902	0.047
6	10.986	20407	2224	0.084
7	11.222	26812	3160	0.110
8	11.536	11105	1335	0.045
9	11.693	12056	1944	0.049
10	11.992	23639163	1157475	96.833
11	13.054	50674	6658	0.208
12	13.317	1559	305	0.006
13	13.528	33992	5468	0.139
14	15.239	1032	101	0.004
15	15.676	3114	454	0.013
16	16.033	1031	251	0.004

Peak#	Ret. Time	Area	Height	Area%
17	16.254	1141	120	0.005
18	17.209	2793	393	0.011
19	21.466	1802	297	0.007
20	21.714	17554	1285	0.072
21	22.278	495033	72682	2.028
22	23.393	8716	1087	0.036
23	23.793	2275	328	0.009
24	24.423	8077	1054	0.033
25	24.874	1433	187	0.006
Total		24412420	1267931	100.000