

Sample Name:β-Endorphin, human
 Cat No. :RP11344
 Lot No. :E4915420K
 Time Processed :11:30:26 PM
 Month-Day-Year Processed :11/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

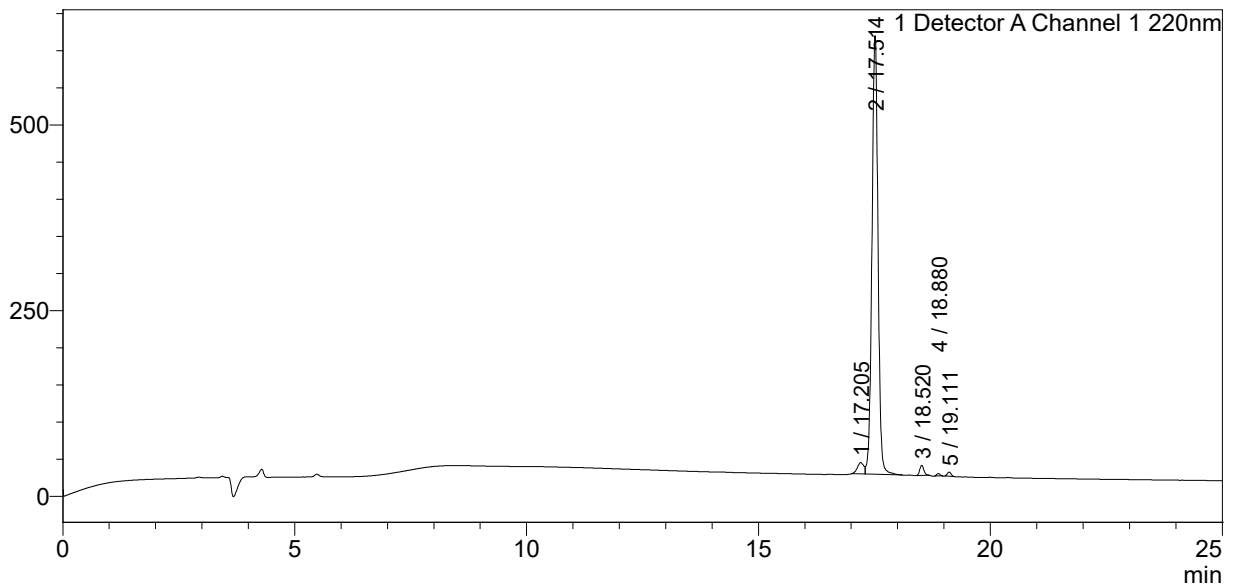

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.205	150653	15266	2.686
2	17.514	5331187	590557	95.063
3	18.520	82100	13481	1.464
4	18.880	14905	3032	0.266
5	19.111	29198	5353	0.521
Total		5608043	627688	100.000