

Sample Name : β -Amyloid (1-42), human
 Cat. No. : RP10017
 Lot. No. : E7770319F
 Time Processed : 17:21:57
 Month-Day-Year Processed : 06/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

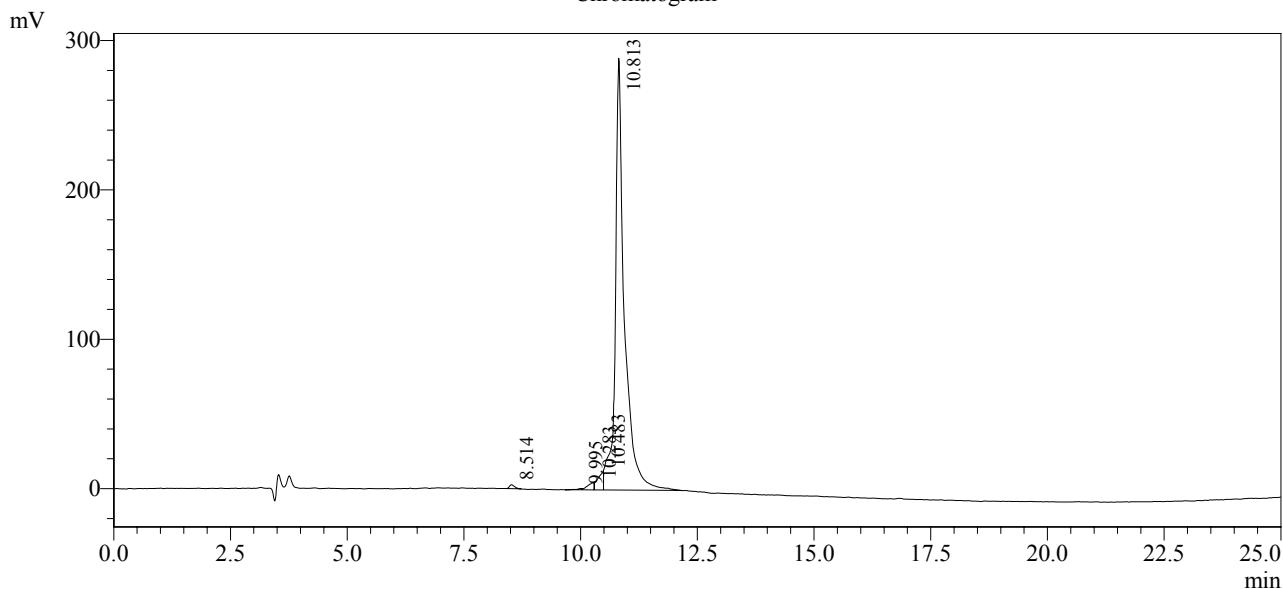

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.514	19590	2598	0.477
2	9.995	6086	884	0.148
3	10.283	46028	4826	1.121
4	10.483	104535	12464	2.547
5	10.813	3928797	289084	95.707
Total		4105035	309854	100.000