

Sample Name : Cys-TAT(47-57)  
 Cat No. : RP20343  
 Lot No. : E8078721C  
 Time Processed : 7:00:18  
 Month-Day-Year Processed : 03/18/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : ZJ20010139

<Chromatogram>

mV

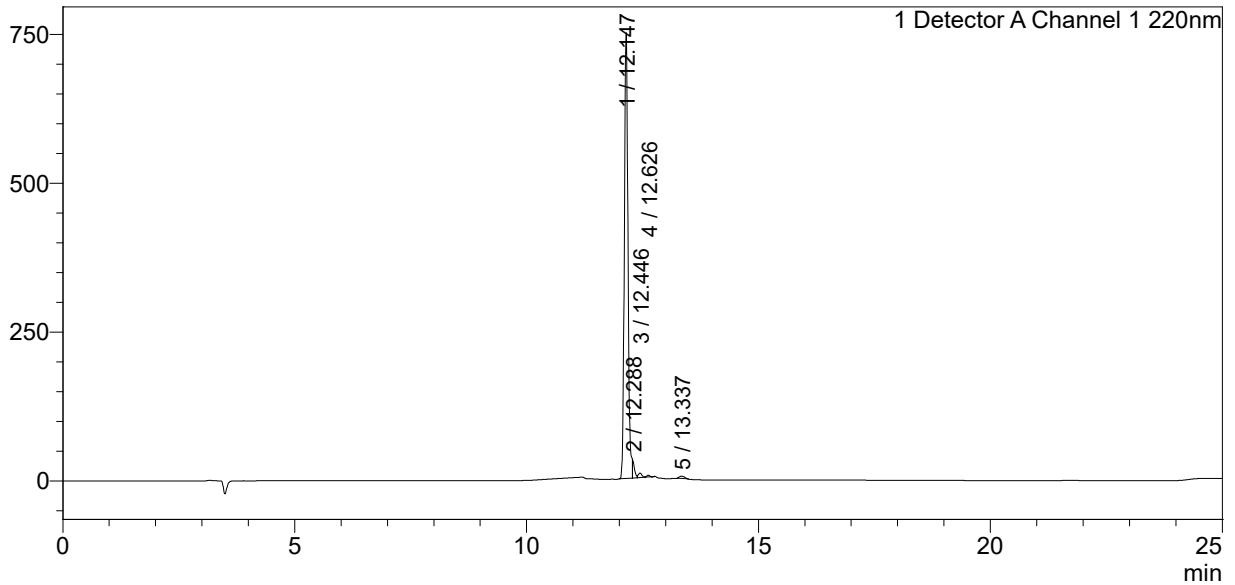

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.147	4118504	748493	96.308
2	12.288	79626	31497	1.862
3	12.446	38966	7529	0.911
4	12.626	8813	2682	0.206
5	13.337	30477	3862	0.713
Total		4276387	794063	100.000