

Sample Name : hgp100(25-33)
 Cat. No. : RP20344
 Lot. No. : PE1821701

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

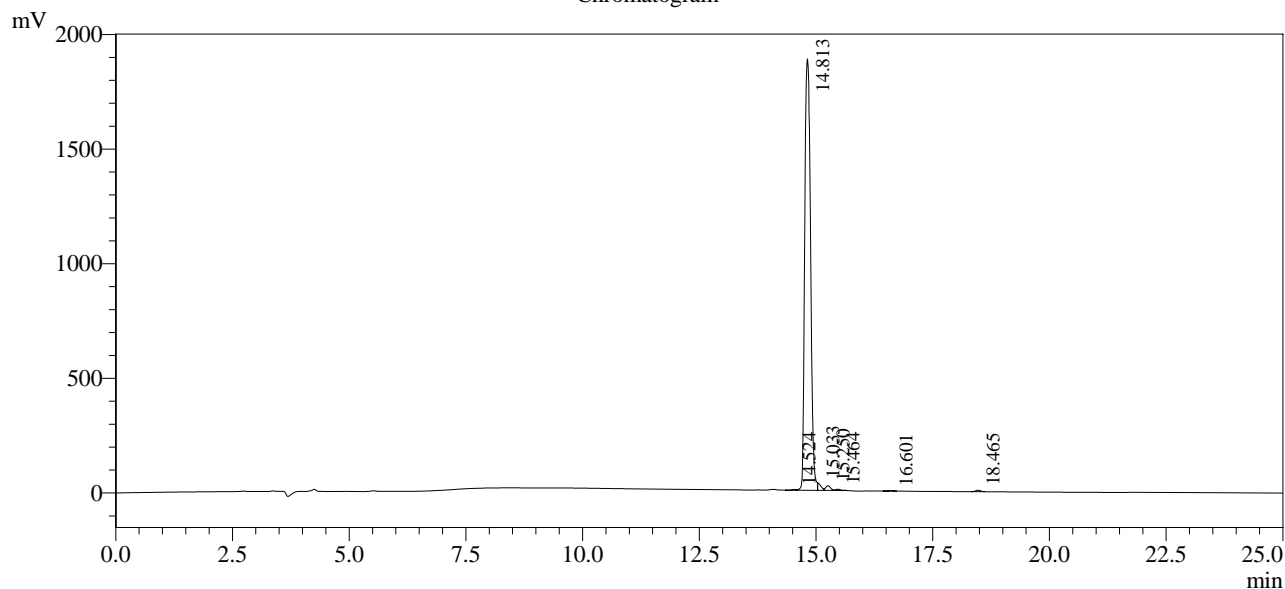

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.524	16857	3258	0.101
2	14.813	16316476	1881978	97.627
3	15.033	146027	32476	0.874
4	15.250	144416	20196	0.864
5	15.464	29005	5123	0.174
6	16.601	14046	2761	0.084
7	18.465	46302	6256	0.277
Total		16713129	1952049	100.000