

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :E4283620L
 Time Processed :9:22:52 PM
 Month-Day-Year Processed :12/26/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

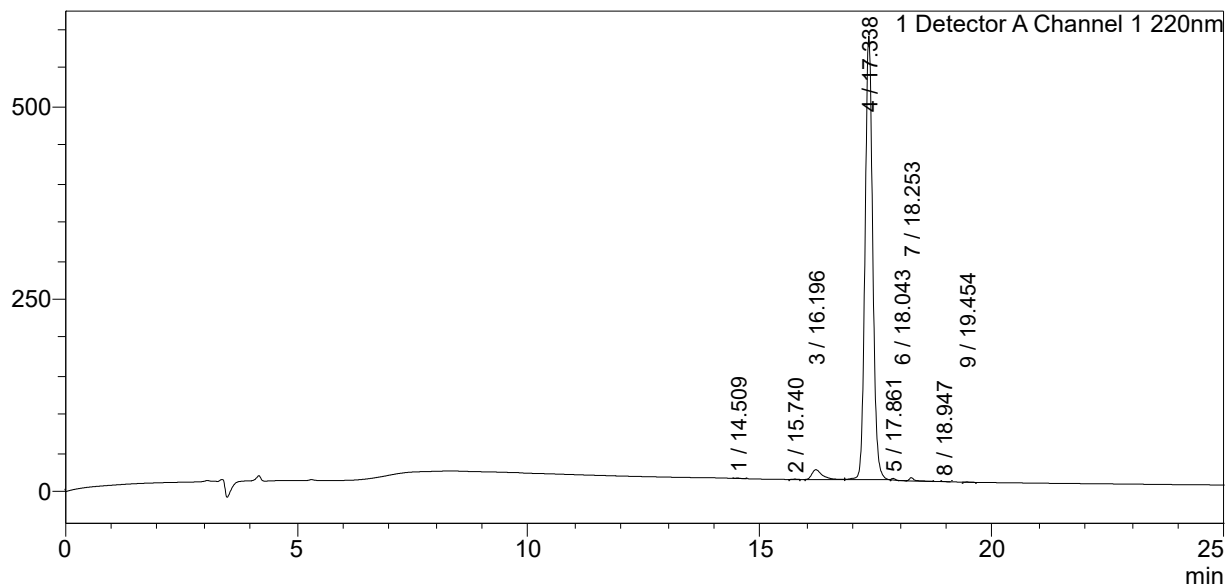

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.509	3000	488	0.044
2	15.740	4567	587	0.067
3	16.196	202499	12745	2.951
4	17.338	6604057	575170	96.256
5	17.861	10455	1970	0.152
6	18.043	1048	235	0.015
7	18.253	32017	4218	0.467
8	18.947	1123	188	0.016
9	19.454	2136	311	0.031
Total		6860903	595912	100.000