

Sample Name :HA Peptide
 Cat No.: RP11735
 Lot No.: E1591919I
 Time Processed :8:18:04
 Month-Day-Year Processed :09/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

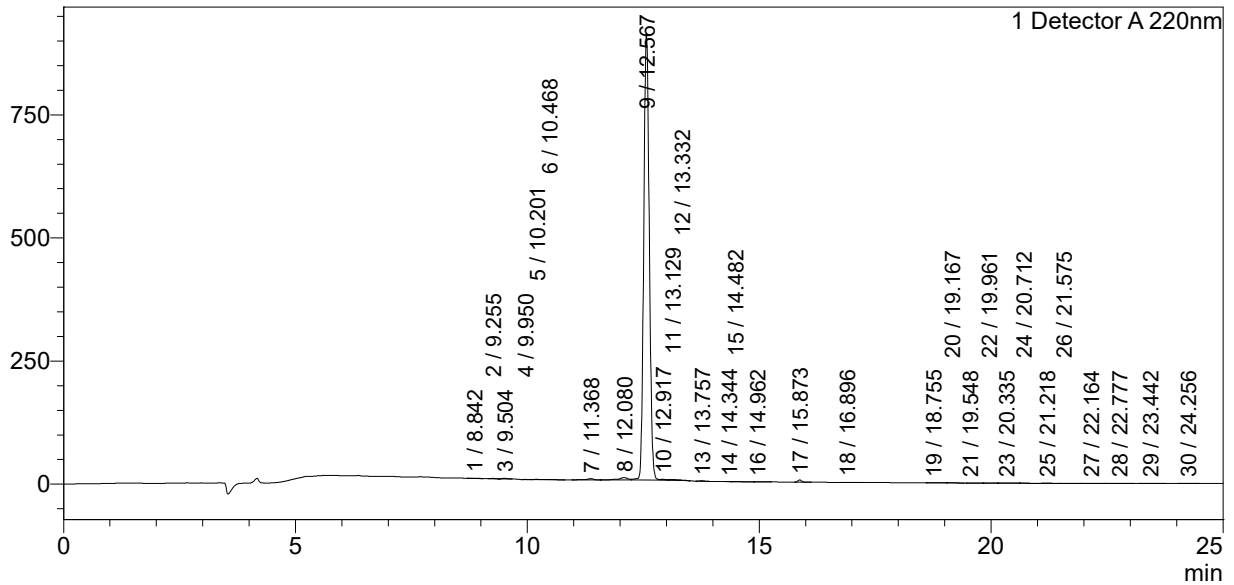

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.842	4272	451	0.055
2	9.255	3488	513	0.045
3	9.504	9124	1390	0.118
4	9.950	1141	187	0.015
5	10.201	3069	479	0.040
6	10.468	2732	188	0.035
7	11.368	31240	2696	0.403
8	12.080	72970	5017	0.940
9	12.567	7545306	908245	97.233
10	12.917	3254	459	0.042
11	13.129	6611	894	0.085
12	13.332	3670	298	0.047
13	13.757	8414	1119	0.108
14	14.344	2069	327	0.027
15	14.482	6237	437	0.080

Peak#	Ret. Time	Area	Height	Area%
16	14.962	2477	295	0.032
17	15.873	25320	4638	0.326
18	16.896	2532	183	0.033
19	18.755	1399	114	0.018
20	19.167	1121	105	0.014
21	19.548	1509	73	0.019
22	19.961	2718	300	0.035
23	20.335	2093	145	0.027
24	20.712	1355	182	0.017
25	21.218	4463	202	0.058
26	21.575	3094	170	0.040
27	22.164	3009	199	0.039
28	22.777	1880	100	0.024
29	23.442	2386	178	0.031
30	24.256	1088	82	0.014
Total		7760042	929669	100.000