

Sample Name :OVA Peptide (323-339)  
 Cat No. : RP10610  
 Lot No. :E6798819J  
 Time Processed : 19:24:52  
 Month-Day-Year Processed : 10/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

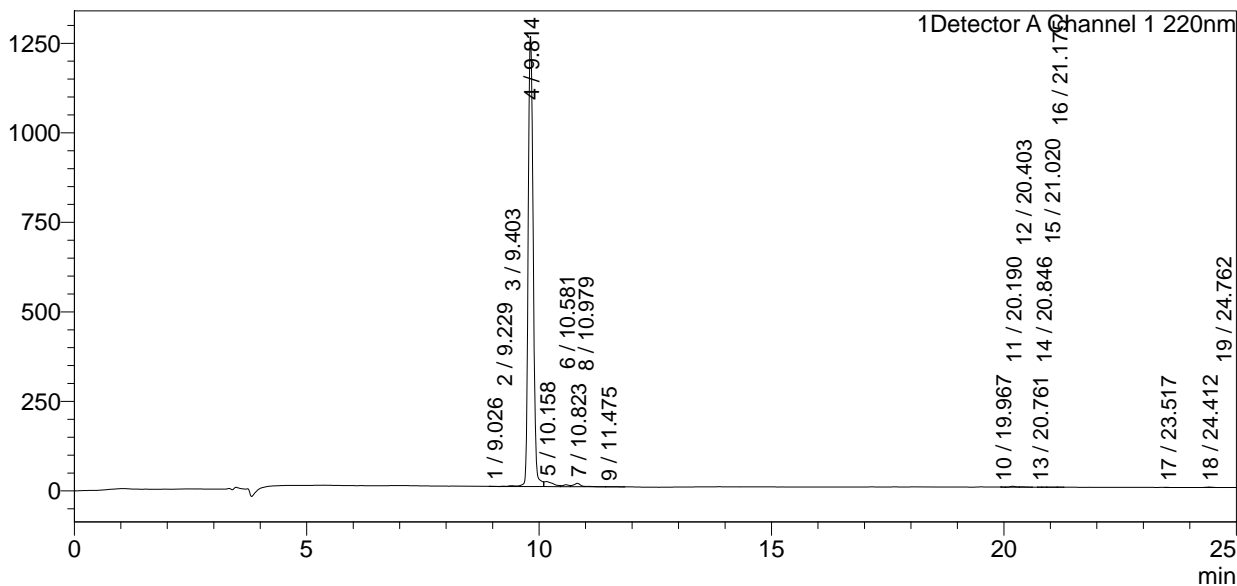

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.026	4381	745	0.045
2	9.229	4810	822	0.049
3	9.403	20893	2200	0.212
4	9.814	9410358	1256807	95.654
5	10.158	187437	14239	1.905
6	10.581	51668	5508	0.525
7	10.823	93740	9575	0.953
8	10.979	15207	1056	0.155
9	11.475	5668	393	0.058
10	19.967	40	17	0.000
11	20.190	20147	2427	0.205
12	20.403	6684	758	0.068
13	20.761	127	52	0.001
14	20.846	100	19	0.001
15	21.020	1097	126	0.011

Peak#	Ret. Time	Area	Height	Area%
16	21.175	317	65	0.003
17	23.517	1224	301	0.012
18	24.412	12487	1138	0.127
19	24.762	1555	160	0.016
Total		9837939	1296409	100.000