

Sample Name :Cys-TAT(47-57)

Cat. No. : RP20343

Lot. No. : PE2561811

Time Processed : 10:14:19

Month-Day-Year Processed :11/08/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:SS-CM-0286

Chromatogram

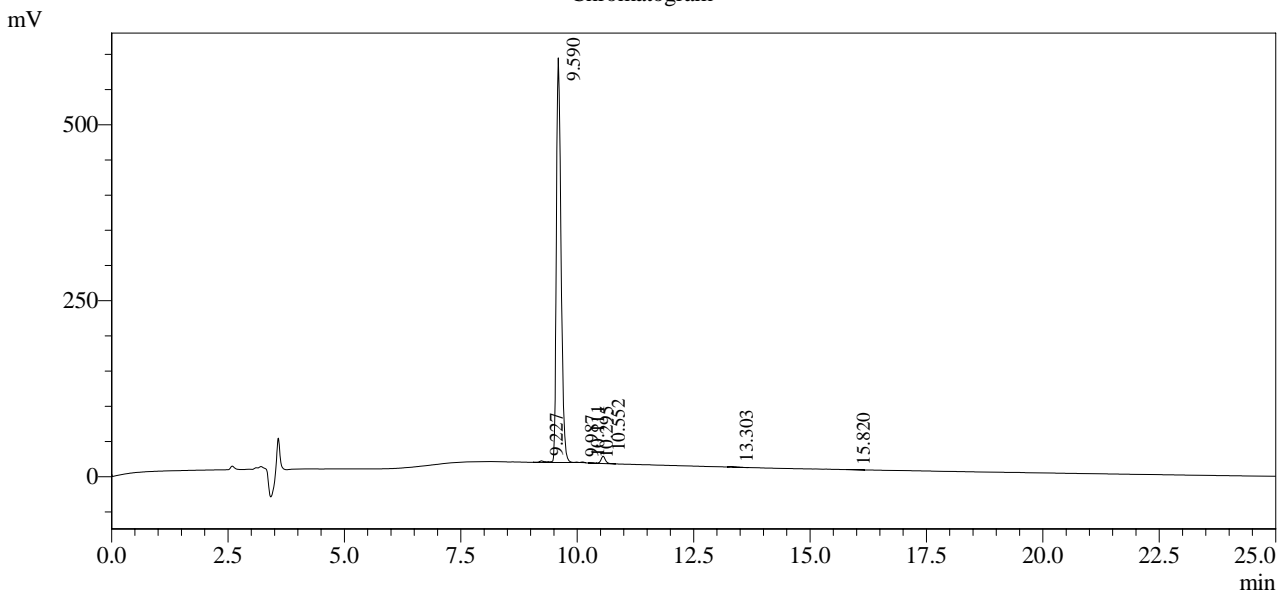

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.227	17071	2142	0.414
2	9.590	4028952	574769	97.630
3	9.987	2799	588	0.068
4	10.111	3191	799	0.077
5	10.295	1674	299	0.041
6	10.552	66691	10257	1.616
7	13.303	5174	565	0.125
8	15.820	1194	94	0.029
Total		4126744	589514	100.000