

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E4750021D
 Time Processed :3:49:15
 Month-Day-Year Processed :04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

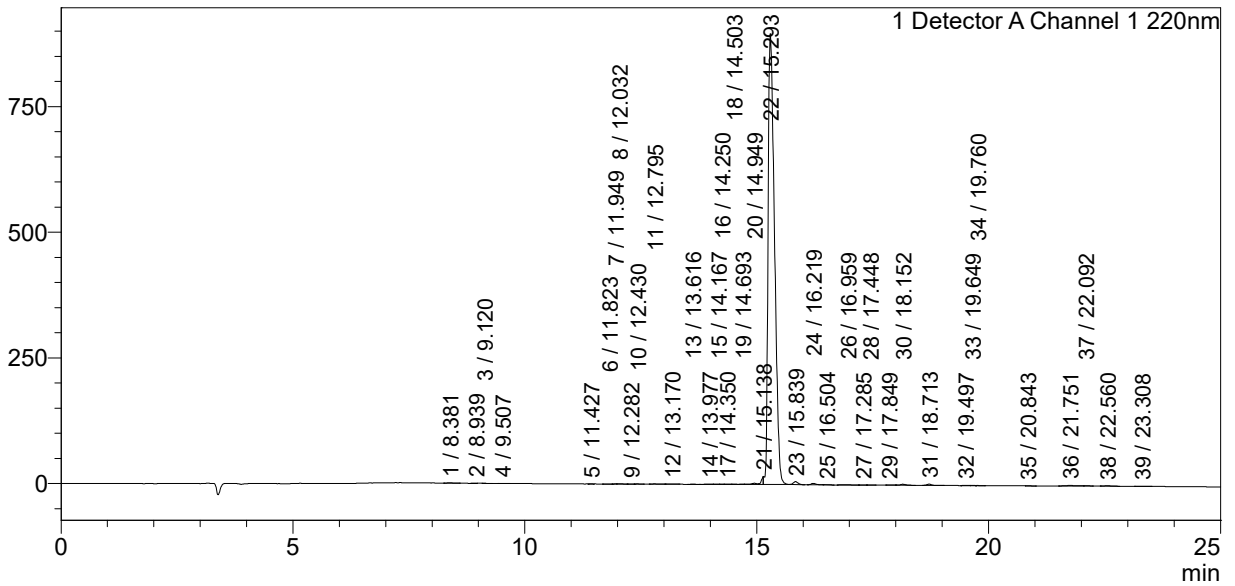

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.381	3369	351	0.038
2	8.939	1054	148	0.012
3	9.120	1125	172	0.013
4	9.507	1415	182	0.016
5	11.427	1018	197	0.011
6	11.823	1849	232	0.021
7	11.949	1597	312	0.018
8	12.032	4154	362	0.047
9	12.282	2502	303	0.028
10	12.430	3191	448	0.036
11	12.795	3863	591	0.043
12	13.170	3947	560	0.044
13	13.616	1943	296	0.022
14	13.977	3980	409	0.045

Peak#	Ret. Time	Area	Height	Area%
15	14.167	2790	404	0.031
16	14.250	2515	441	0.028
17	14.350	3536	403	0.040
18	14.503	2288	324	0.026
19	14.693	2657	436	0.030
20	14.949	21624	2214	0.243
21	15.138	43955	14682	0.494
22	15.293	8629640	897121	97.068
23	15.839	38903	5759	0.438
24	16.219	19981	2838	0.225
25	16.504	1615	245	0.018
26	16.959	6694	482	0.075
27	17.285	1142	209	0.013
28	17.448	1975	317	0.022
29	17.849	1275	176	0.014
30	18.152	15108	1979	0.170
31	18.713	18579	2450	0.209
32	19.497	2067	278	0.023
33	19.649	1152	185	0.013
34	19.760	1050	204	0.012
35	20.843	1267	138	0.014
36	21.751	19308	1017	0.217
37	22.092	3458	404	0.039
38	22.560	7785	1037	0.088
39	23.308	4905	446	0.055
Total		8890276	938749	100.000