

Sample Information

Sample Name :CGRP (8-37), rat
 Cat. No :RP11090
 Lot. No. :PE5351805

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

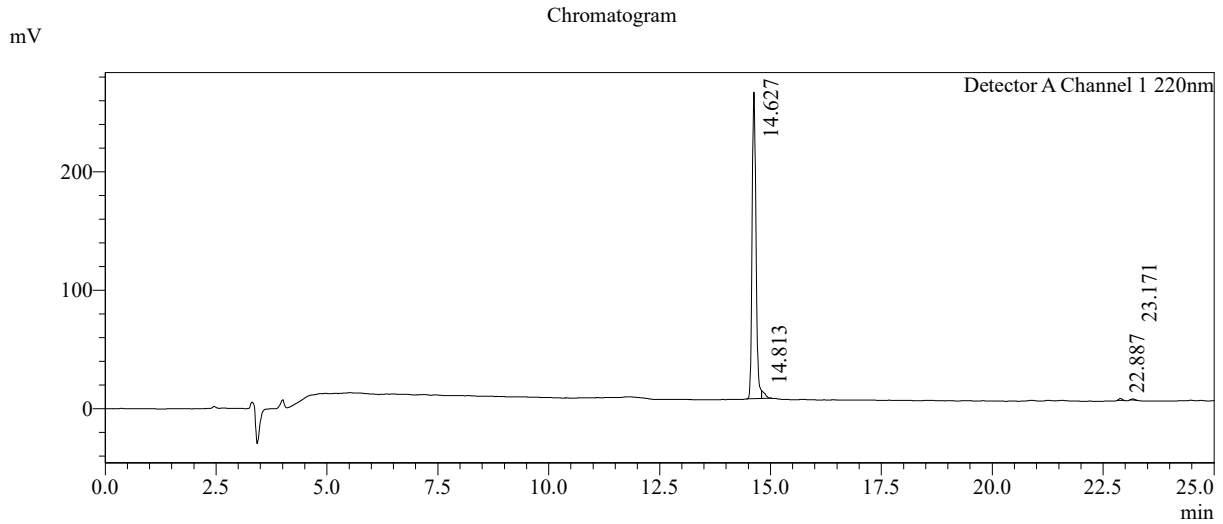

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	14.627	258539	1575033	96.697	97.203
2	14.813	6277	32125	2.348	1.983
3	22.887	1618	8246	0.605	0.509
4	23.171	936	4947	0.350	0.305
Total		267369	1620351	100.000	100.000