

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : PE8861901
 Time Processed :3:37:07
 Month-Day-Year Processed : 01/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

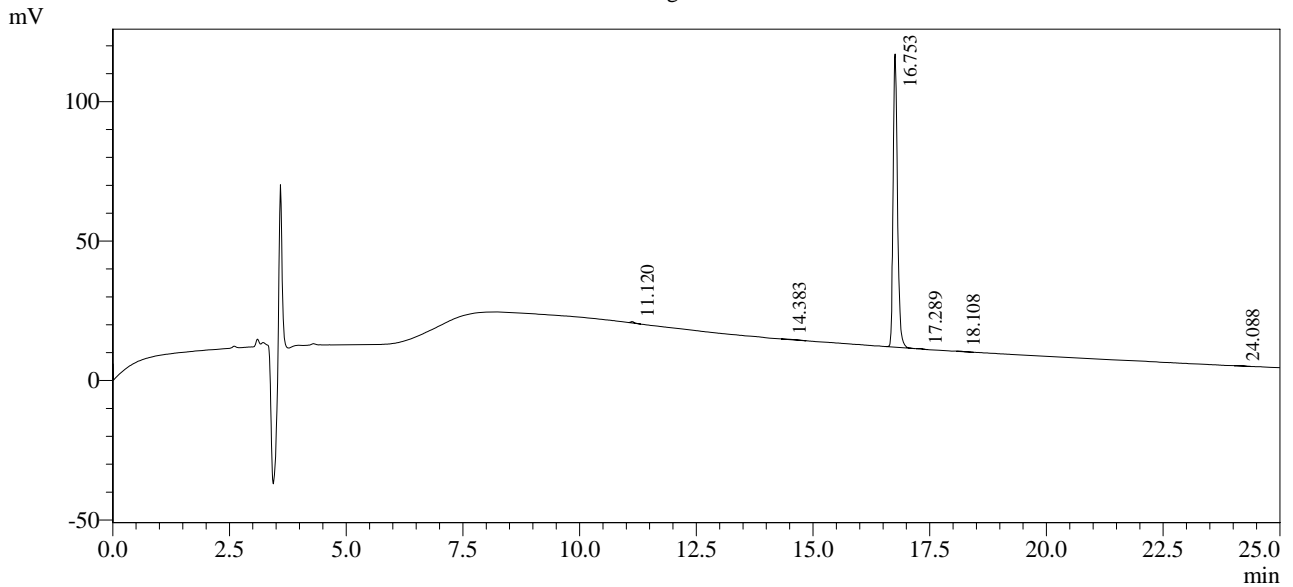

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.120	2587	480	0.372
2	14.383	3465	178	0.499
3	16.753	684875	105164	98.593
4	17.289	1158	168	0.167
5	18.108	1371	111	0.197
6	24.088	1194	96	0.172
Total		694649	106197	100.000