

Sample Name :SV40 T-Ag-derived NLS peptide  
 Cat. No. : RP20513  
 Lot. No. :PE2551612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

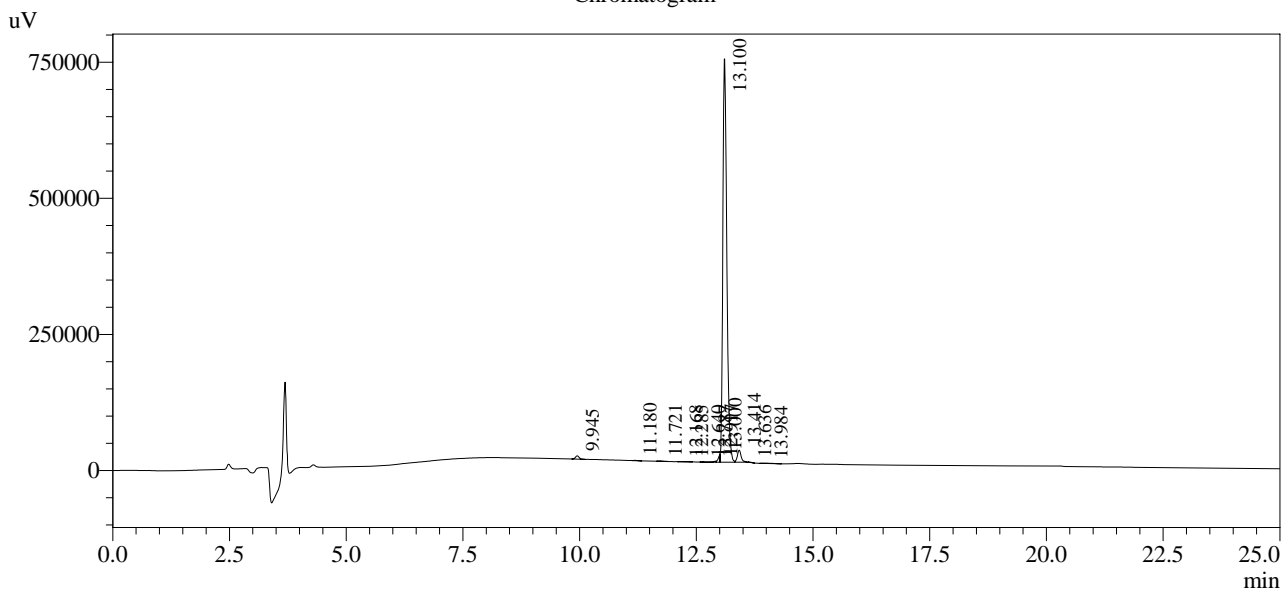

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.945	31811	5988	0.691
2	11.180	3133	597	0.068
3	11.721	3863	725	0.084
4	12.168	1898	404	0.041
5	12.285	3427	657	0.074
6	12.640	1718	420	0.037
7	12.787	2081	516	0.045
8	12.917	5986	1937	0.130
9	13.000	38510	12860	0.836
10	13.100	4378210	740607	95.051
11	13.414	124397	22087	2.701
12	13.636	1958	488	0.043
13	13.984	9157	544	0.199
Total		4606149	787828	100.000