

Sample Name : $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : E3440020G  
 Time Processed : 14:03:57  
 Month-Day-Year Processed : 09/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Boston Green C4 4.6 x 250 mm  
 Equipment : SS-CM-0310

Chromatogram

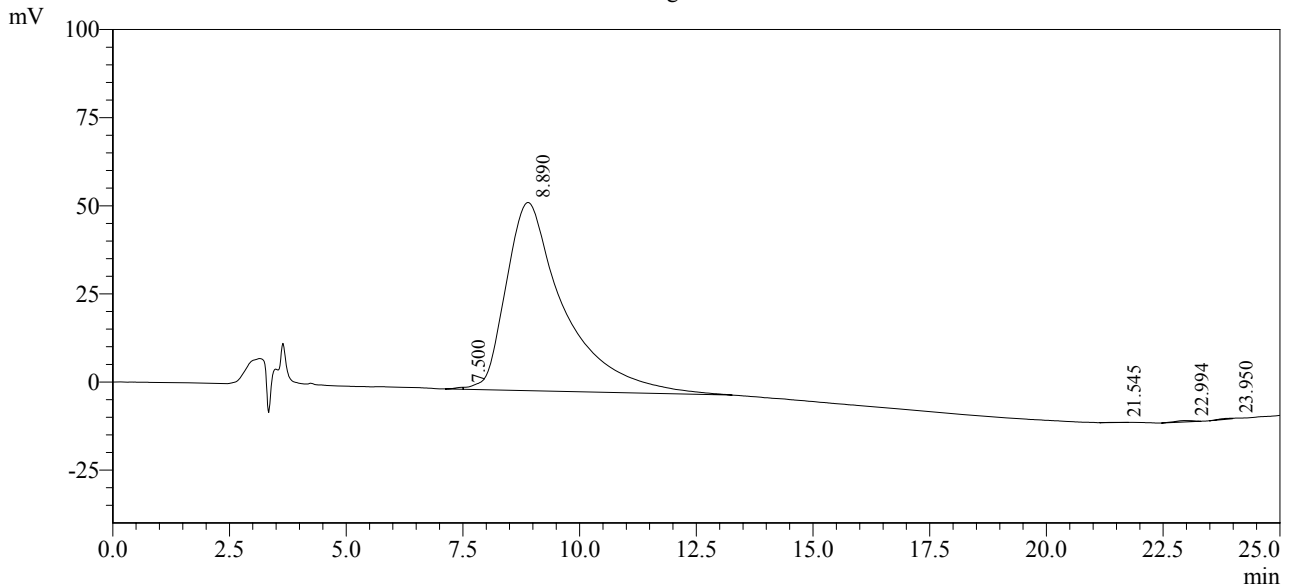

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.500	6666	570	0.142
2	8.890	4654136	53402	99.484
3	21.545	1611	78	0.034
4	22.994	10408	376	0.222
5	23.950	5477	195	0.117
Total		4678297	54620	100.000