Mass Spectrum

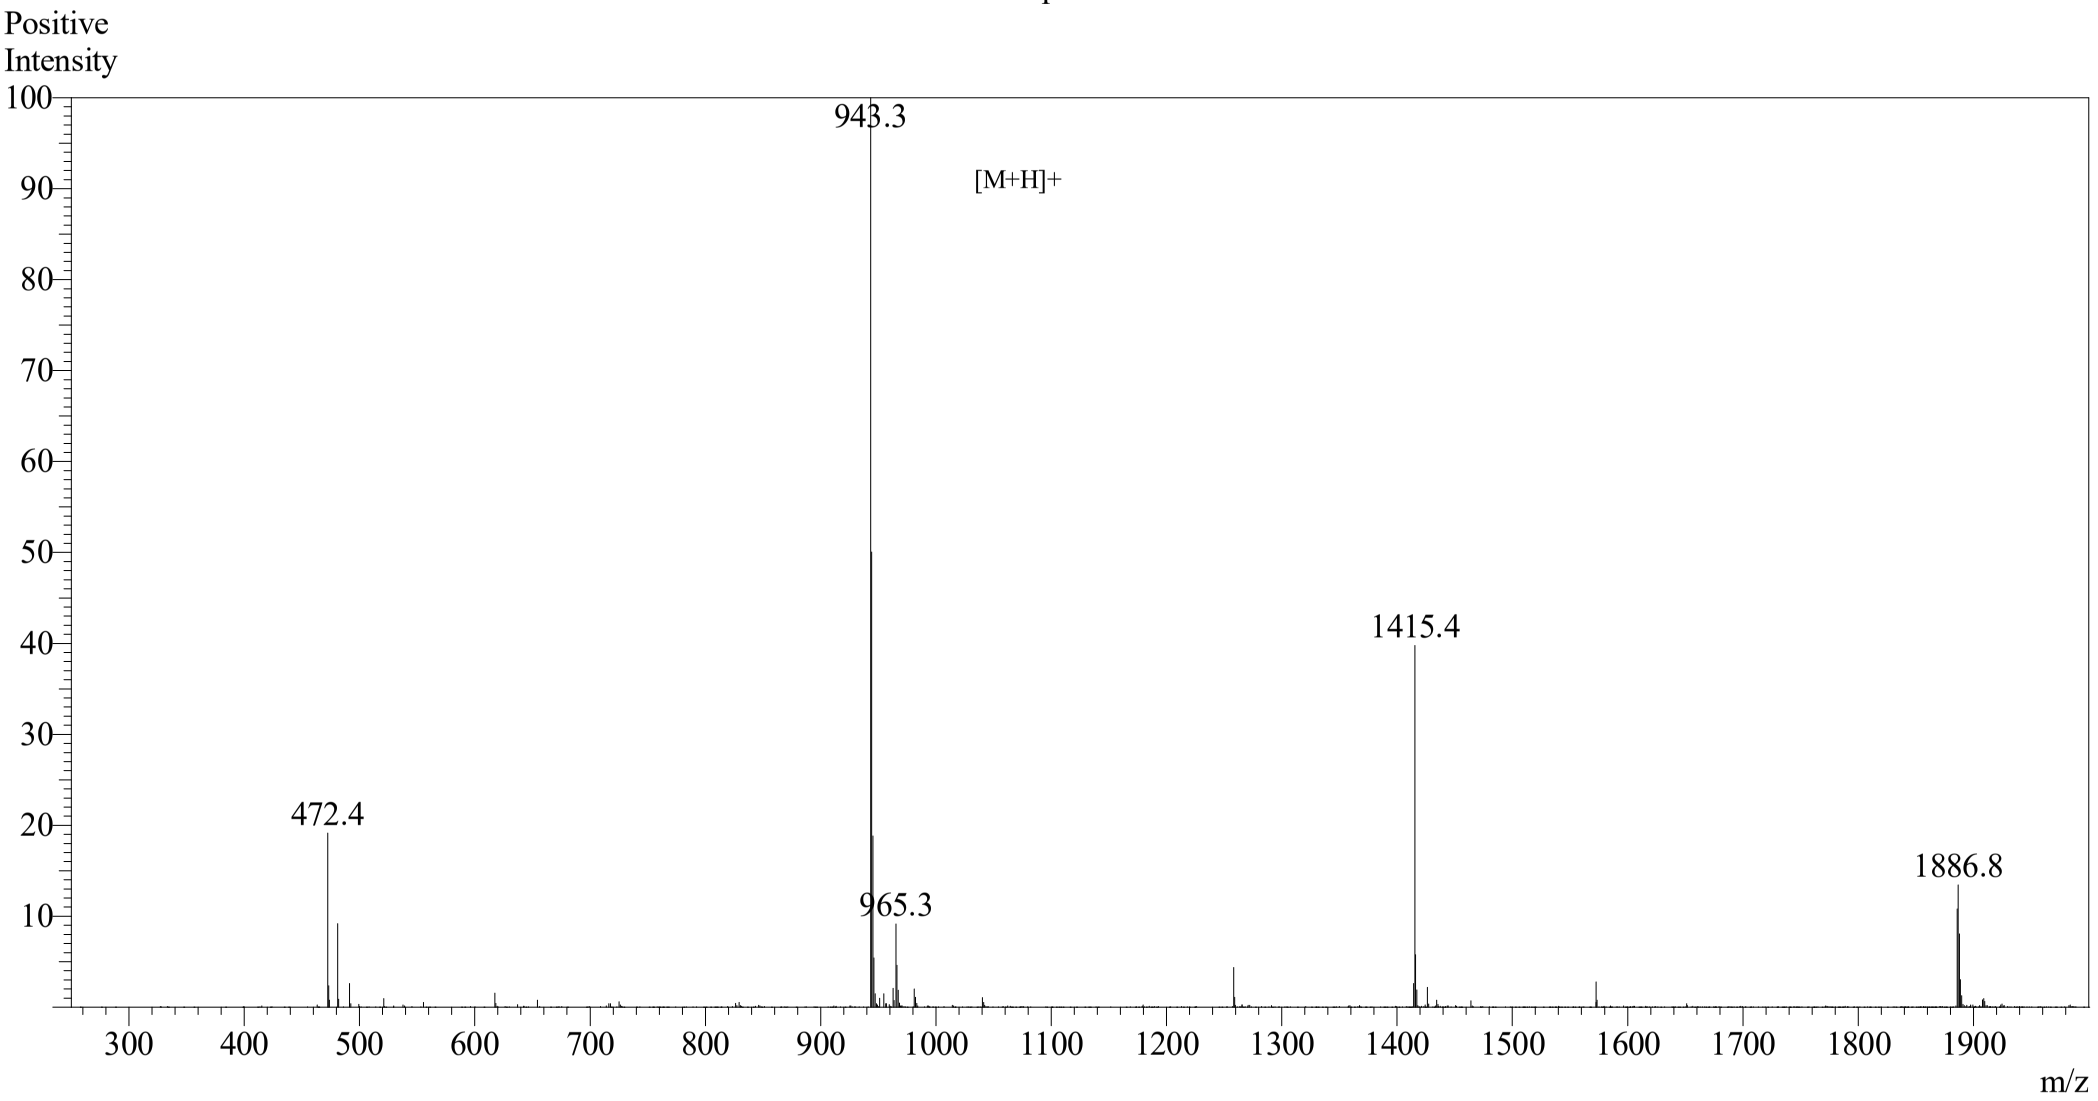

Sample Information
Month-Day Processed : 12/22/20
Time Processed : 8:40:52 PM
Injection Volume : 0.4
Sample Name : CEF20
Cat No. : RP11781
Lot No. : E7892720L
Theoretical MW : 943.18
Observed MW : 942.3

Interface :ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH