

Sample Name :LL37 (Human)
 Cat No. :RP13323
 Lot No. :E8052221A
 Time Processed :22:16:49
 Month-Day-Year Processed :01/06/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

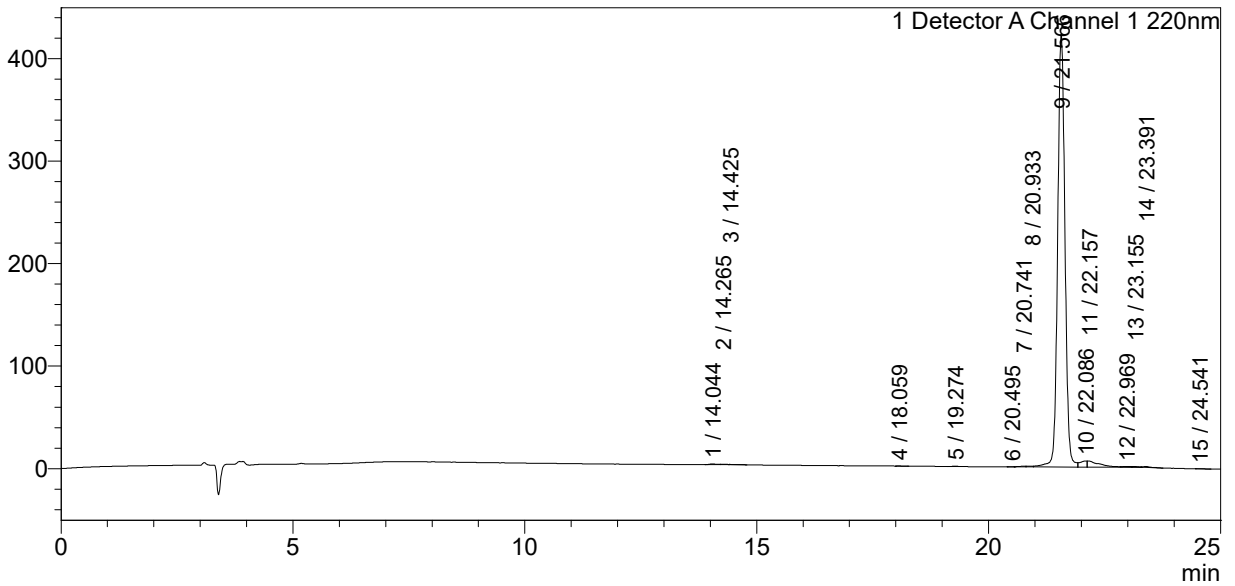

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.044	9562	879	0.198
2	14.265	3952	422	0.082
3	14.425	4026	315	0.083
4	18.059	1041	125	0.022
5	19.274	3888	512	0.081
6	20.495	1216	171	0.025
7	20.741	7326	671	0.152
8	20.933	7194	829	0.149
9	21.566	4606453	423066	95.388
10	22.086	61520	5761	1.274
11	22.157	105204	5763	2.179
12	22.969	5332	503	0.110
13	23.155	2975	431	0.062
14	23.391	7918	770	0.164

Peak#	Ret. Time	Area	Height	Area%
15	24.541	1590	156	0.033
Total		4829197	440373	100.000